
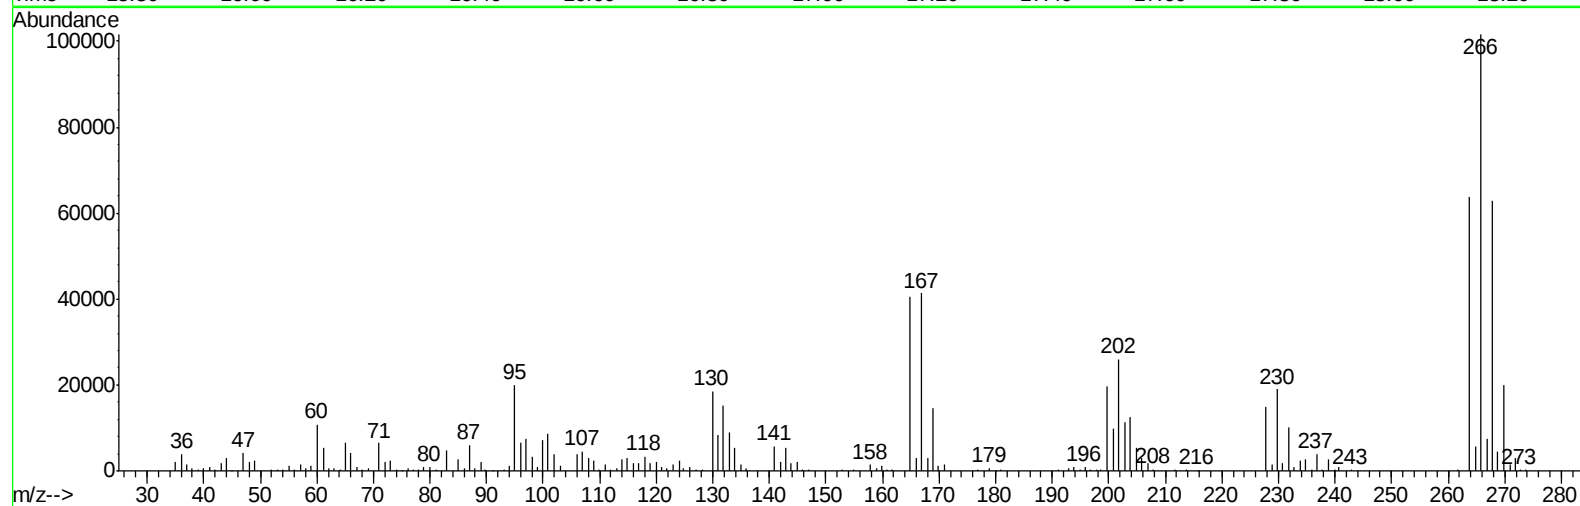


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071219\
Data File : BG041632.D
Acq On : 12 Jul 2019 9:50
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 23:31:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:39:06 2019
Response via : Initial Calibration

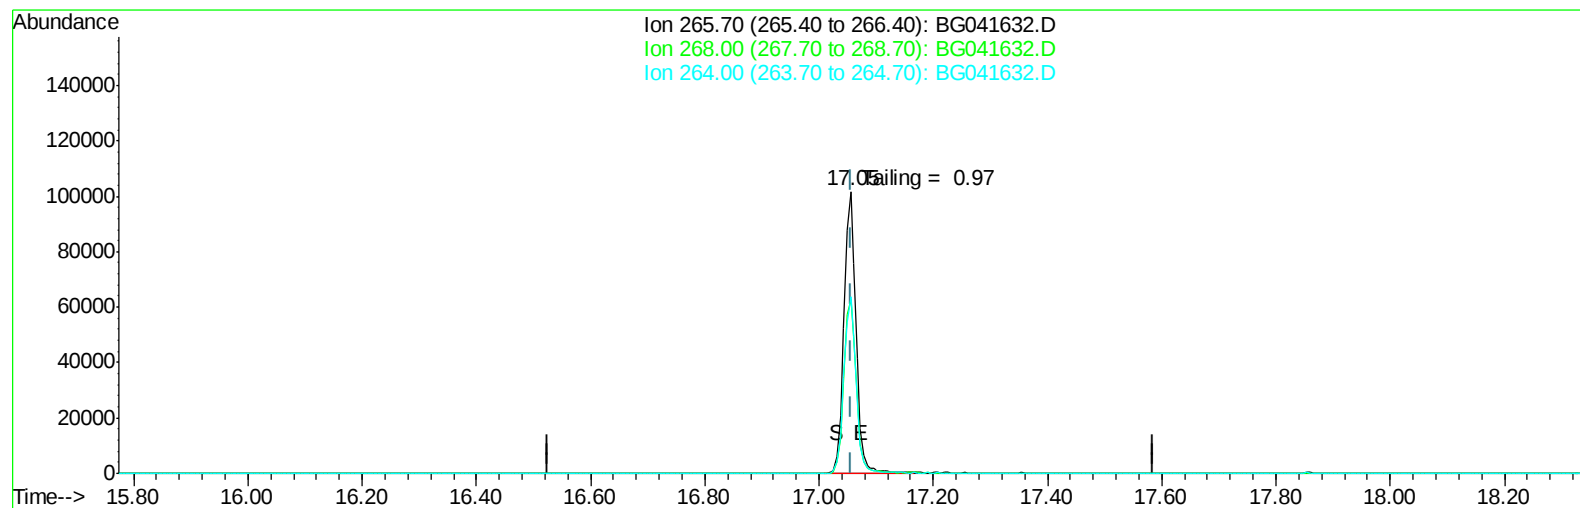

TIC: BG041632.D

(70) Pentachlorophenol (C)



17.055min (-0.001) -20.00ng

response 149259

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.02
264.00	64.00	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071219\
Data File : BG041632.D
Acq On : 12 Jul 2019 9:50
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 23:31:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:39:06 2019
Response via : Initial Calibration

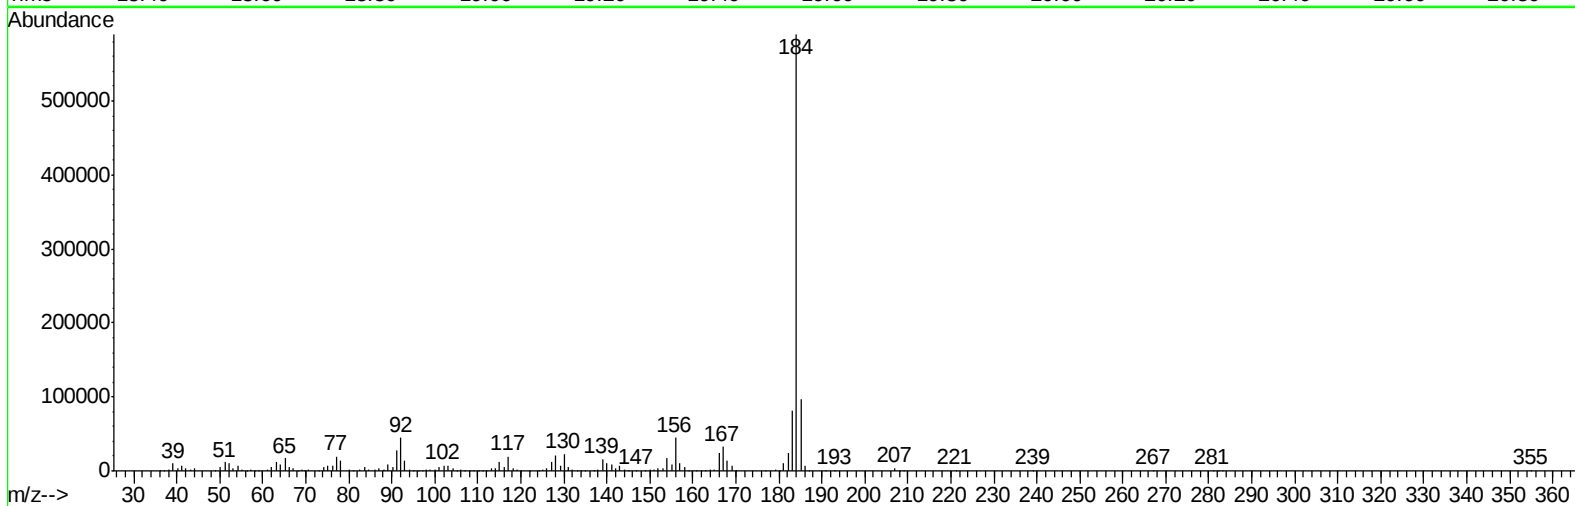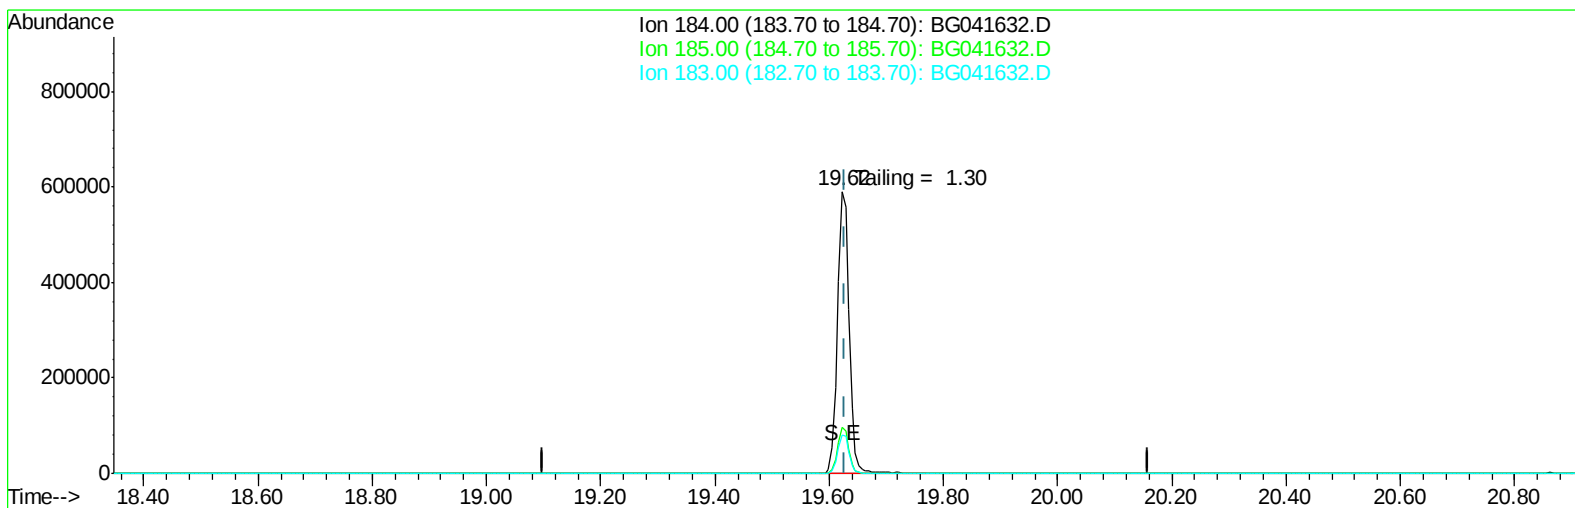

TIC: BG041632.D

(77) Benzidine

19.622min (-0.007) 182427.65ng

response 827087

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	16.53
183.00	12.00	13.82
0.00	0.00	0.00