

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071219\
 Data File : BG041638.D
 Acq On : 12 Jul 2019 13:40
 Operator : HP/JU
 Sample : K3636-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP19-MMW0018B

Quant Time: Jul 12 15:36:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:39:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	86421	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	338600	20.00	ng	0.00
39) Acenaphthene-d10	14.67	164	218790	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	526397	20.00	ng	0.00
76) Chrysene-d12	21.66	240	516427	20.00	ng	0.00
87) Perylene-d12	24.86	264	579410	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	330347	64.15	ng	0.00
7) Phenol-d6	7.20	99	292519	41.93	ng	0.00
23) Nitrobenzene-d5	9.21	82	518090	93.25	ng	0.00
42) 2,4,6-Tribromophenol	16.15	330	344534	137.71	ng	0.00
45) 2-Fluorobiphenyl	13.30	172	1310380	94.16	ng	0.00
79) Terphenyl-d14	20.01	244	2056785	97.34	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071219\
Data File : BG041638.D
Acq On : 12 Jul 2019 13:40
Operator : HP/JU
Sample : K3636-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP19-MMW0018B

Quant Time: Jul 12 15:36:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:39:06 2019
Response via : Initial Calibration

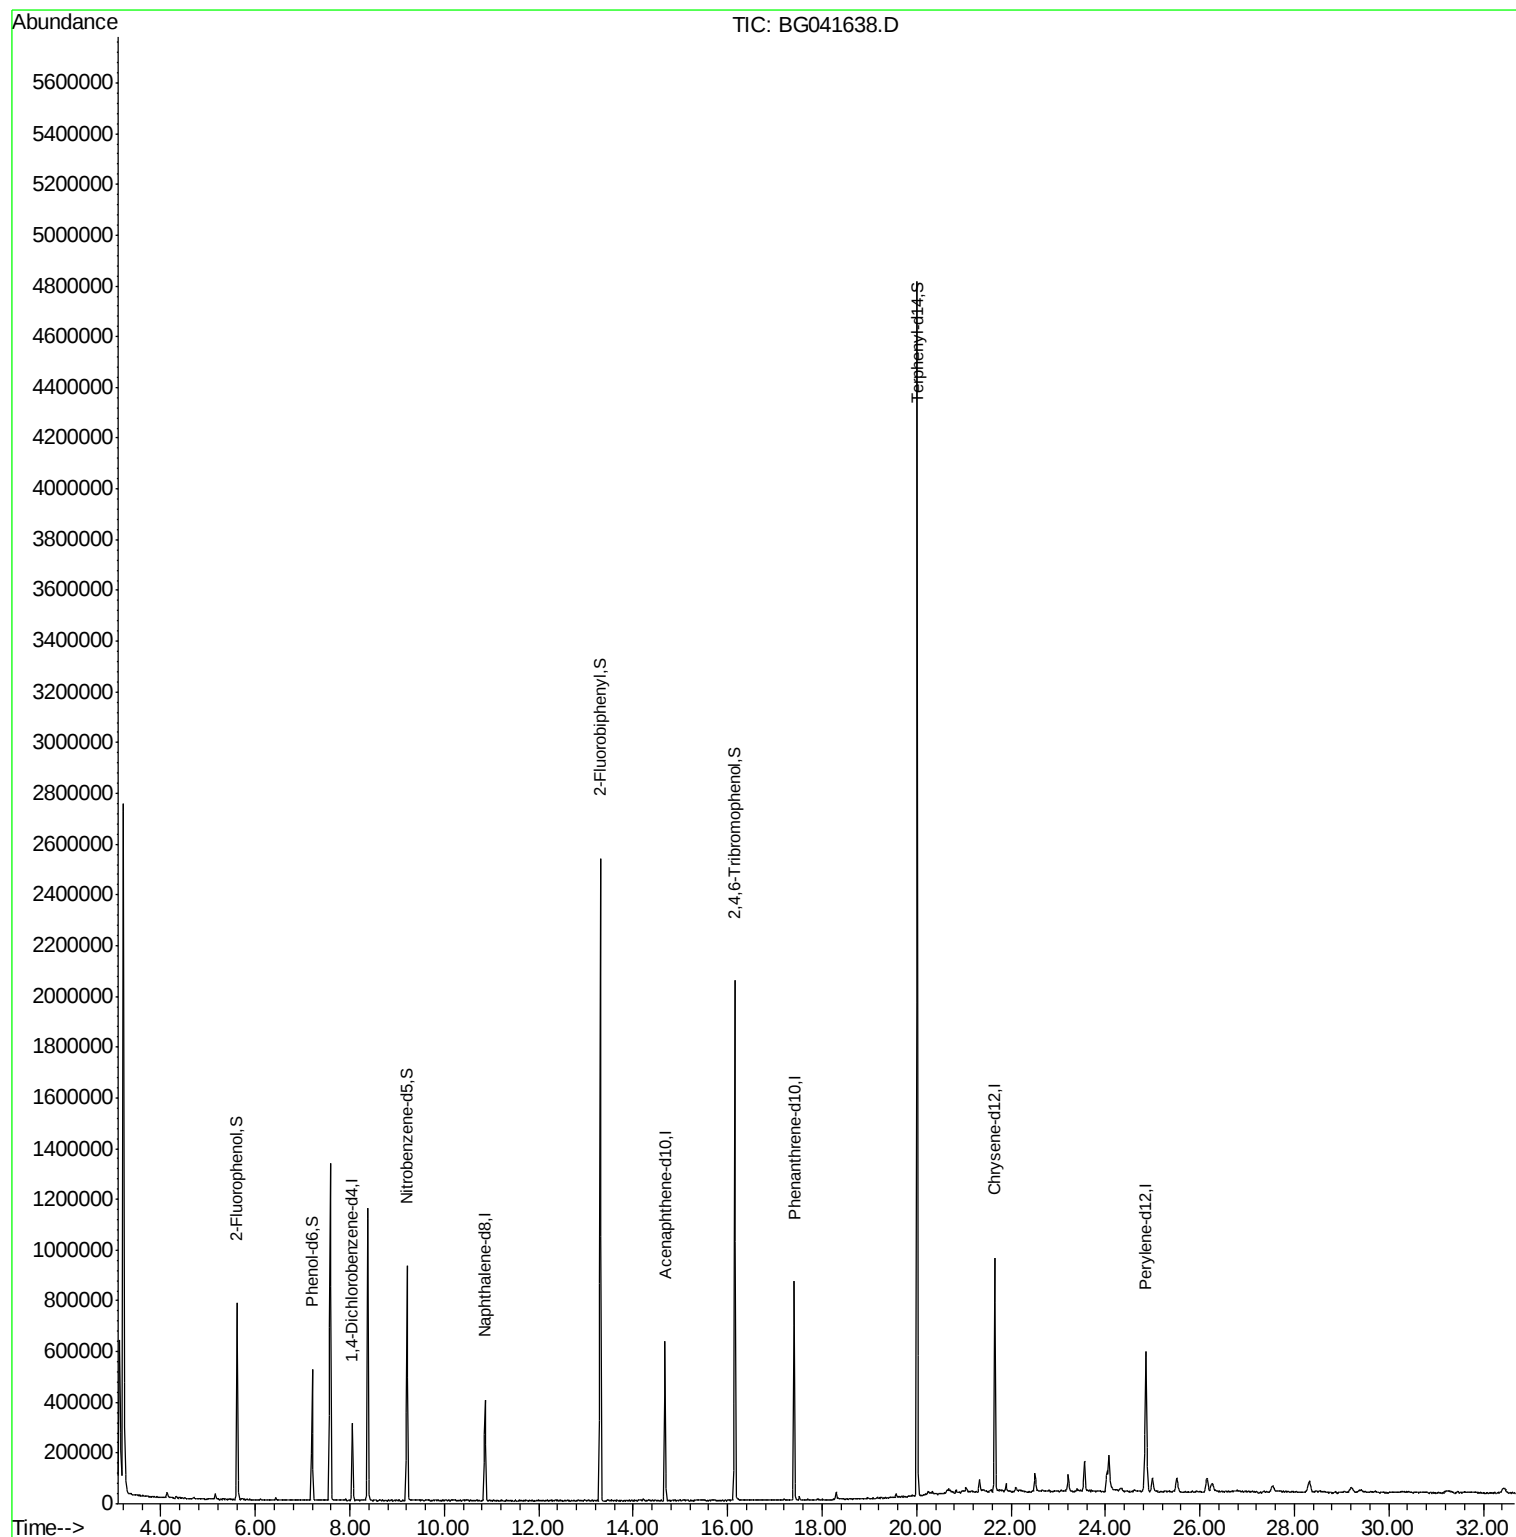




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 845
Delta R.T. -0.00 min
Lab File: BG041638.D
Acq: 12 Jul 2019 13:40

Instrument :
BNA_G
ClientSampleId :
SP19-MMW0018B

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.0	120.6	181.0
115	54.9	47.9	71.9



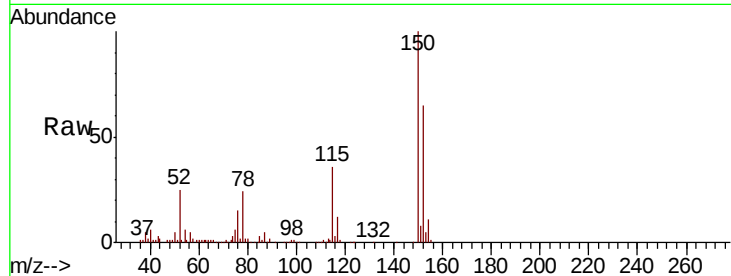


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

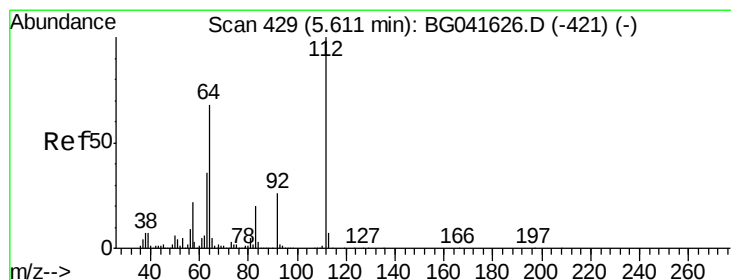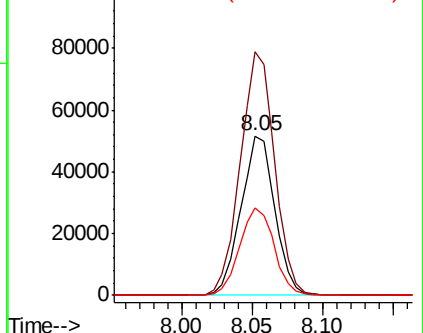

#5

2-Fluorophenol
Concen: 64.145 ng
RT: 5.61 min Scan# 430
Delta R.T. 0.00 min
Lab File: BG041638.D
Acq: 12 Jul 2019 13:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.4	55.9	83.9
63	35.7	34.6	51.8






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

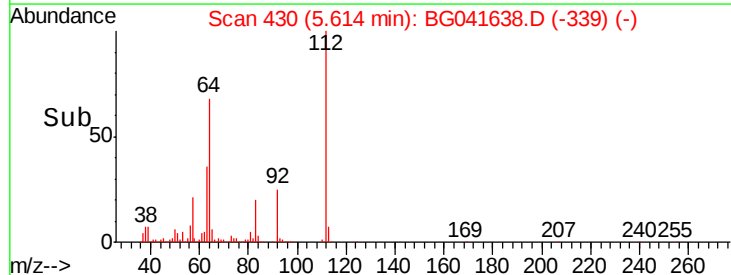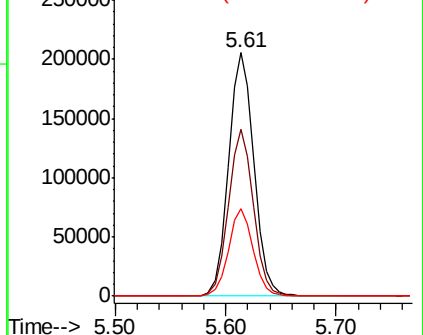



#7

Phenol-d6

Concen: 41.926 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.00 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40

Instrument :

BNA_G

ClientSampleId :

SP19-MMW0018B


Tot Ion: 99 Resp: 292519

Ion Ratio Lower Upper




99 100

42 21.8 19.9 29.9

71 33.6 36.4 54.6#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

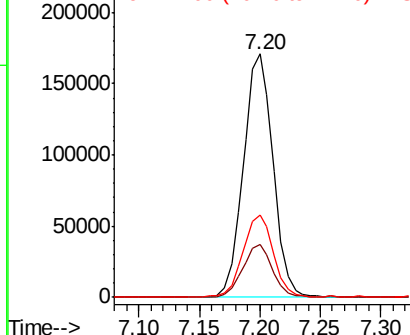

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.00 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40

Tgt Ion: 136 Resp: 338600


Ion Ratio Lower Upper

136 100



137 10.9 8.8 13.2


54 11.1 6.4 9.6#

68 7.0 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




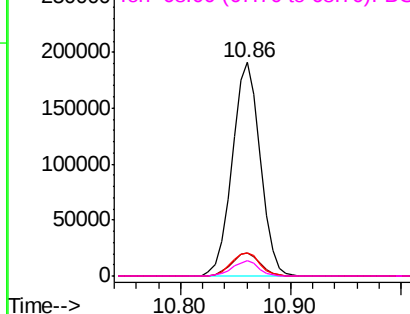




#23
 Nitrobenzene-d5
 Concen: 93.250 ng
 RT: 9.21 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BG041638.D
 Acq: 12 Jul 2019 13:40




Instrument :
 BNA_G
 ClientSampleId :
 SP19-MMW0018B


Tot Ion:	82	Resp:	518090
Ion	Ratio	Lower	Upper
82	100		
128	43.8	29.2	43.8
54	61.8	43.4	65.0

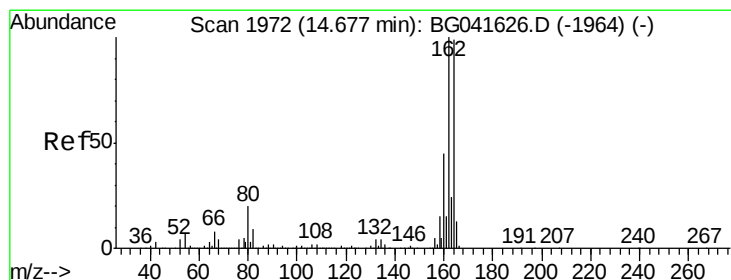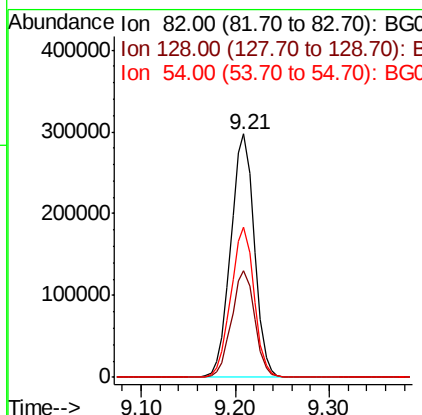

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.67 min Scan# 1972
 Delta R.T. -0.00 min
 Lab File: BG041638.D
 Acq: 12 Jul 2019 13:40

Tgt Ion:	164	Resp:	218790
Ion	Ratio	Lower	Upper
164	100		
162	102.2	82.8	124.2
160	45.7	35.8	53.8

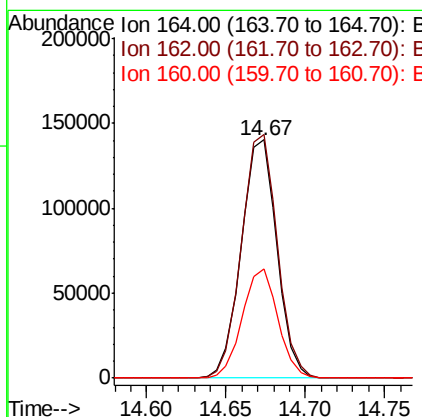

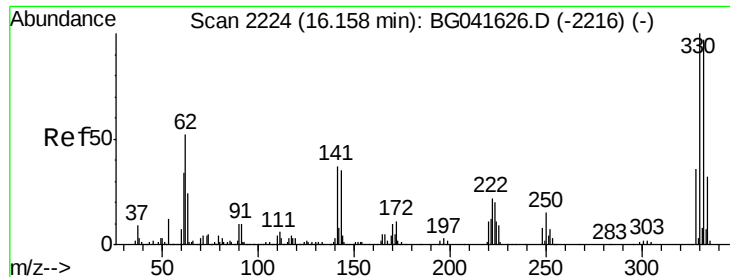

#42

2,4,6-Tribromophenol

Concen: 137.708 ng

RT: 16.15 min Scan# 2223

Delta R.T. -0.01 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40

Instrument :

BNA_G

ClientSampleId :

SP19-MMW0018B


Tot Ion:330 Resp: 344534

Ion Ratio Lower Upper

330 100

332 95.0 75.5 113.3

141 40.4 29.0 43.4



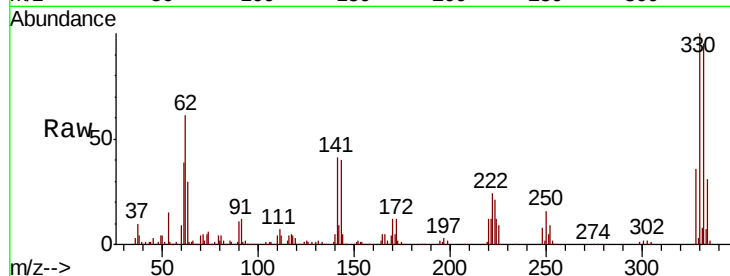


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

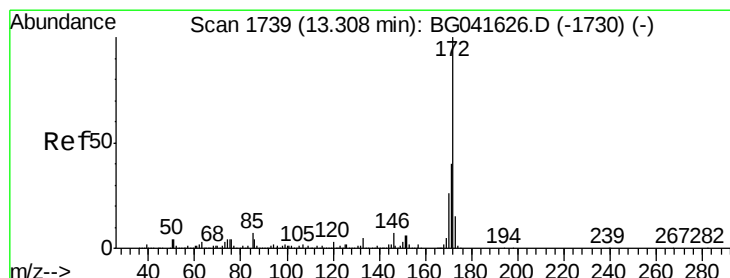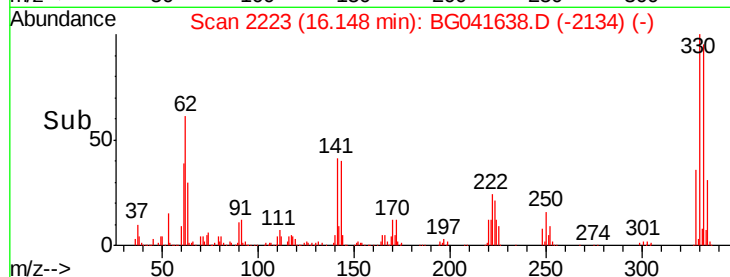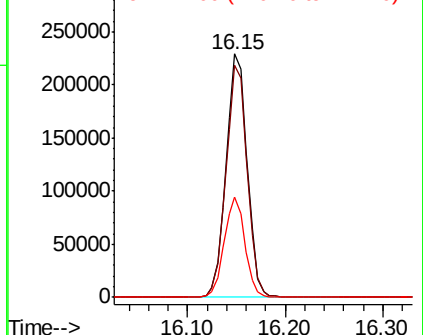

#45

2-Fluorobiphenyl

Concen: 94.159 ng

RT: 13.30 min Scan# 1739

Delta R.T. -0.00 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40


Tgt Ion:172 Resp: 1310380

Ion Ratio Lower Upper

172 100

171 40.3 30.0 45.0

170 26.9 19.8 29.6


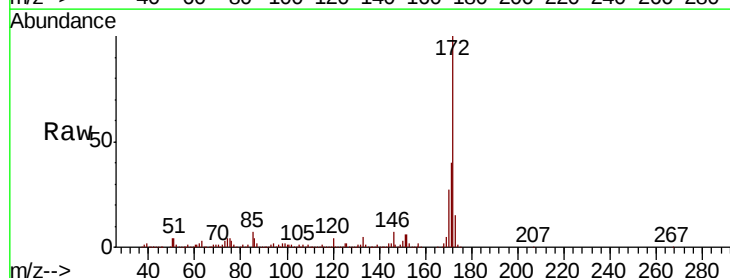



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

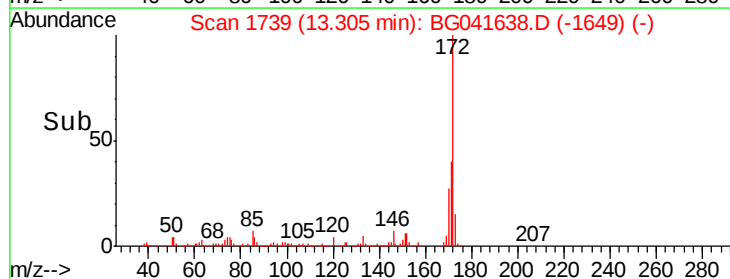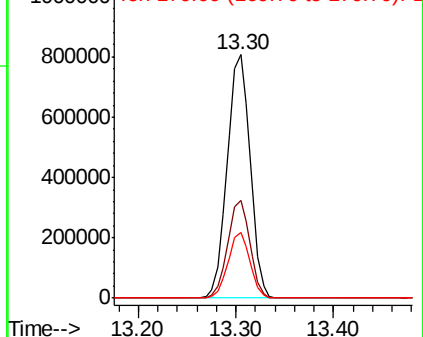



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2437

Delta R.T. -0.01 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40

Instrument :

BNA_G

ClientSampleId :

SP19-MMW0018B


Tot Ion:188 Resp: 526397

Ion Ratio Lower Upper

188 100

94 8.3 3.6 5.4#




80 9.5 4.8 7.2#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

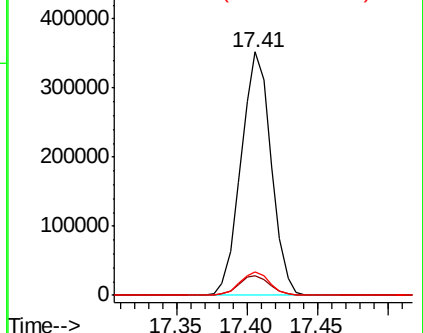

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.66 min Scan# 3161

Delta R.T. -0.01 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40


Tgt Ion:240 Resp: 516427

Ion Ratio Lower Upper

240 100

120 9.6 3.7 5.5#



236 26.8 21.1 31.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

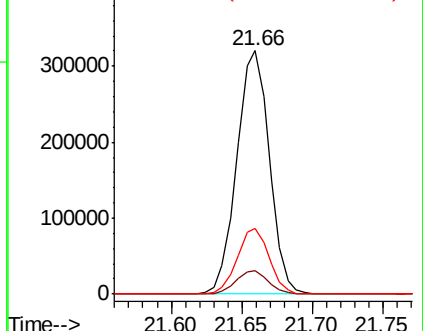



#79

Terphenyl-d14

Concen: 97.340 ng

RT: 20.01 min Scan# 2881

Delta R.T. -0.00 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40

Instrument :

BNA_G

ClientSampleId :

SP19-MMW0018B


Tot Ion:244 Resp: 2056785

Ion Ratio Lower Upper

244 100

212 10.2 6.6 10.0#




122 13.0 5.0 7.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

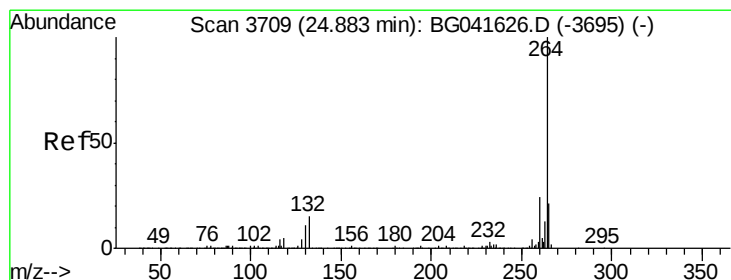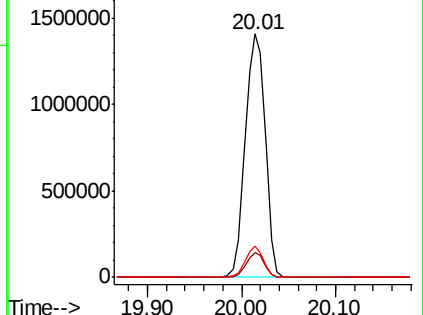

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.86 min Scan# 3705

Delta R.T. -0.03 min

Lab File: BG041638.D

Acq: 12 Jul 2019 13:40


Tgt Ion:264 Resp: 579410

Ion Ratio Lower Upper

264 100

260 23.5 17.4 26.2

265 21.4 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

