


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071219\
Data File : BG041632.D
Acq On : 12 Jul 2019 9:50
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 12 05:39:06 2019

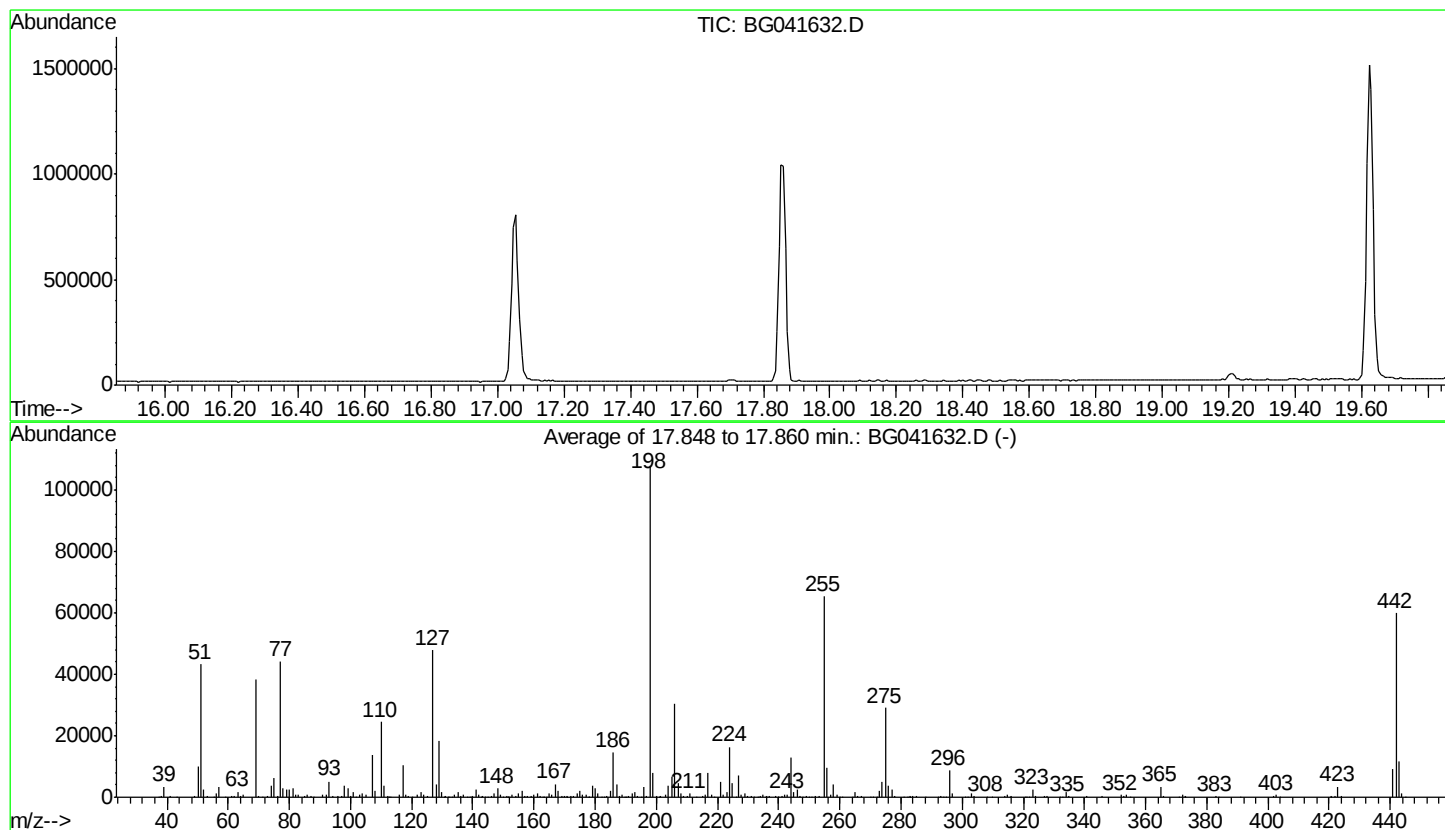

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	43286	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	38520	PASS
70	69	0.00	2	0.9	346	PASS
127	198	10	80	44.4	47848	PASS
197	198	0.00	2	0.3	315	PASS
198	198	100	100	100.0	107872	PASS
199	198	5	9	7.3	7882	PASS
275	198	10	60	26.9	28984	PASS
365	198	1	100	3.1	3393	PASS
441	198	0.01	100	8.7	9356	PASS
442	198	50	100	55.5	59880	PASS
443	442	15	24	19.2	11490	PASS