

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
 Data File : BG049322.D
 Acq On : 13 Jul 2021 20:26
 Operator : CG/JU
 Sample : M2996-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AW8

Quant Time: Jul 14 03:28:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 09 03:15:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.068	152	28357	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.883	136	119201	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.714	164	88789	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	208733	20.000	ng/ul	-0.01
79) Chrysene-d12	21.741	240	212404	20.000	ng/ul	-0.01
88) Perylene-d12	25.025	264	216825	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.456	96	2640	4.379	ng/uL	-0.01
4) Pyridine-d5	3.897	84	6053	3.415	ng/ul	0.01
7) Phenol-d5	7.216	99	15116	6.128	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	39152	27.367	ng/ul	0.00
11) 2-Chlorophenol-d4	7.593	132	39780	21.821	ng/ul	-0.01
15) 4-Methylphenol-d8	8.768	113	28756	14.550	ng/ul	-0.01
21) Nitrobenzene-d5	9.232	128	26644	29.129	ng/ul	0.00
24) 2-Nitrophenol-d4	9.960	143	30090	28.656	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.507	165	55999	27.332	ng/ul	0.00
31) 4-Chloroaniline-d4	11.018	131	50147	18.781	ng/ul	0.00
46) Dimethylphthalate-d6	14.108	166	212527	31.124	ng/ul	0.00
49) Acenaphthylene-d8	14.402	160	239372	29.877	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.907	143	6711	5.938	ng/ul	0.00
60) Fluorene-d10	15.701	176	181642	31.419	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.812	200	25644	19.329	ng/ul	-0.01
73) Anthracene-d10	17.557	188	330153	34.740	ng/ul	-0.01
81) Pyrene-d10	19.843	212	382271	35.114	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.808	264	394240	34.978	ng/ul	-0.01
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.199	77	3170	2.136	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
Data File : BG049322.D
Acq On : 13 Jul 2021 20:26
Operator : CG/JU
Sample : M2996-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AW8


Quant Time: Jul 14 03:28:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 09 03:15:38 2021
Response via : Initial Calibration

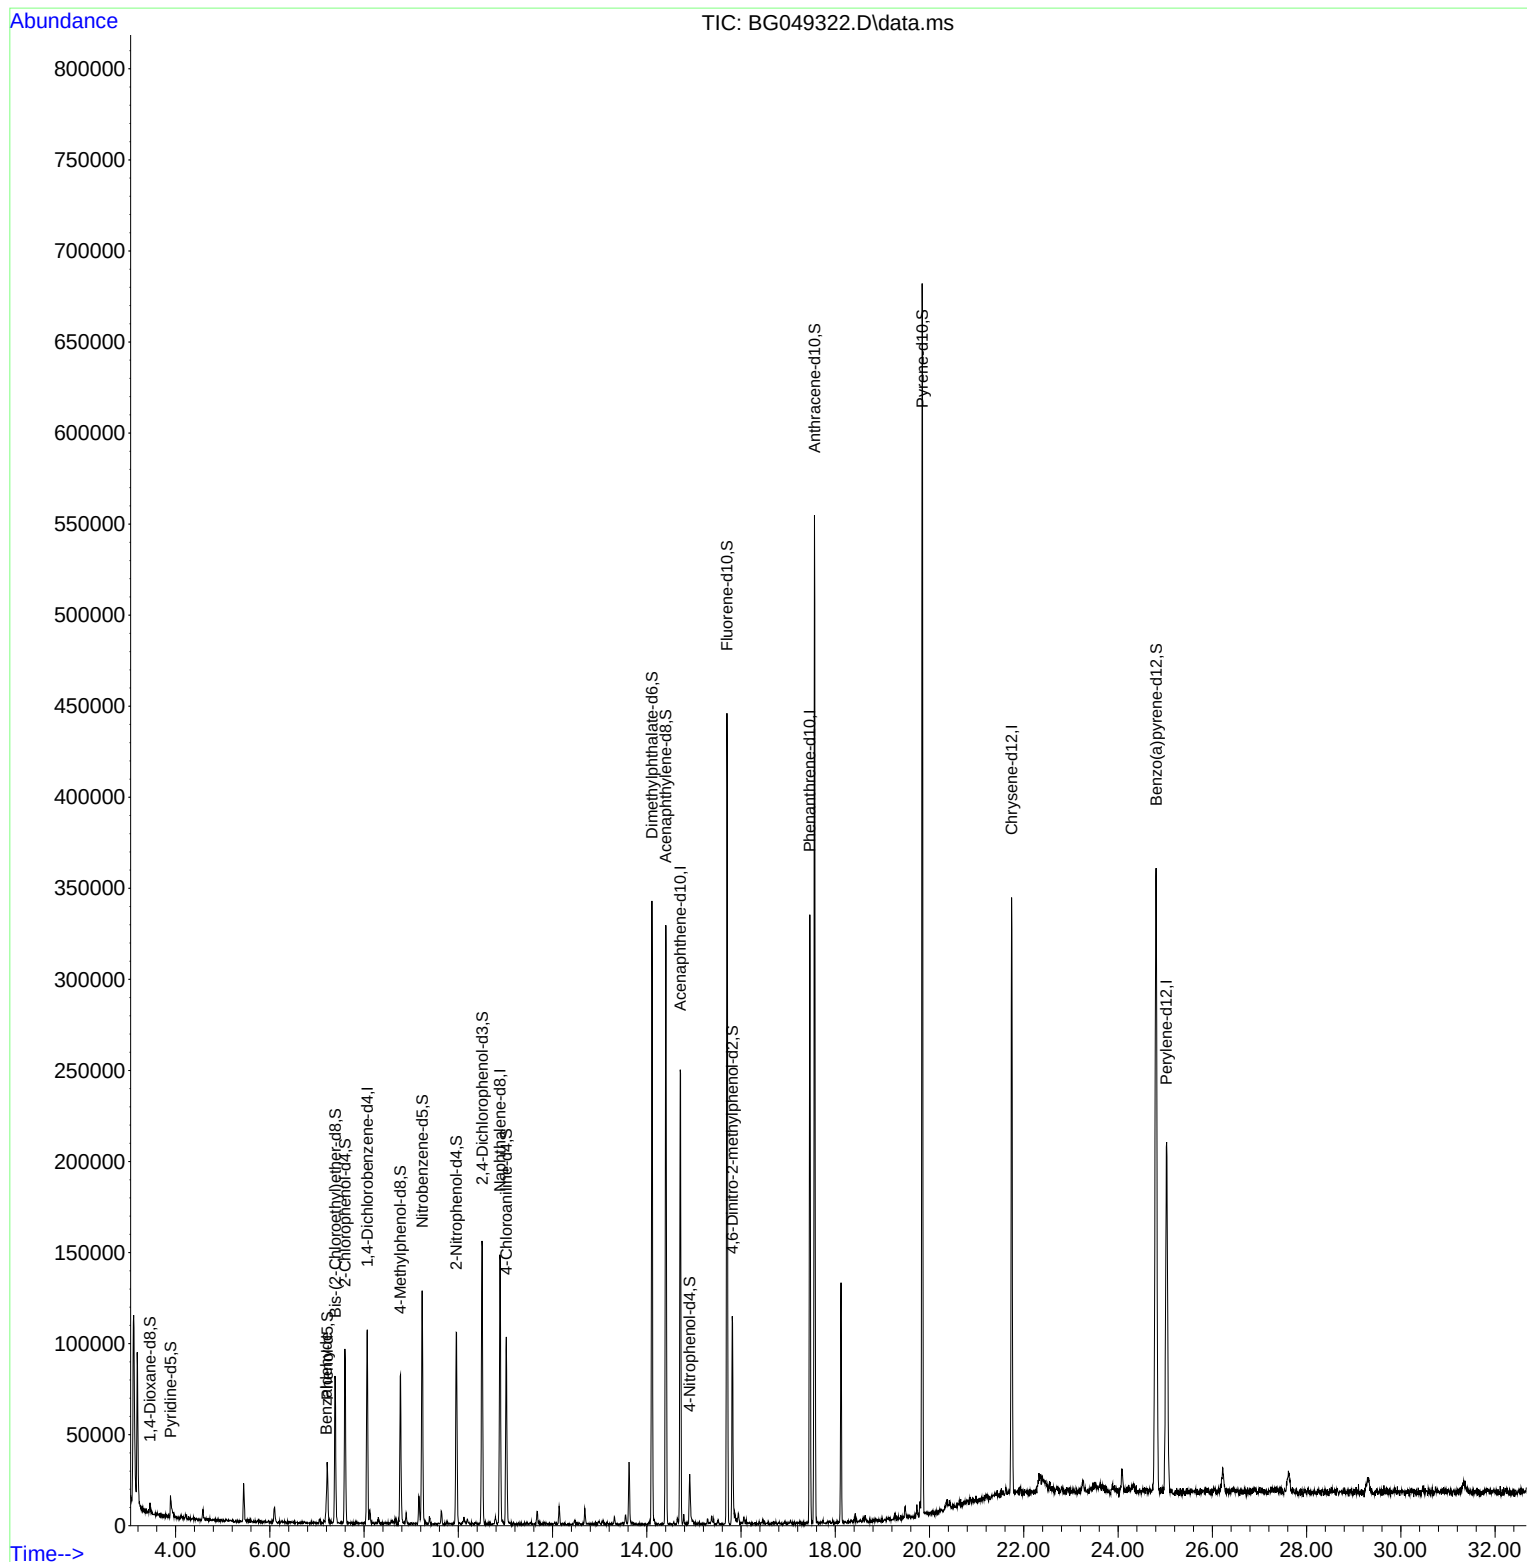

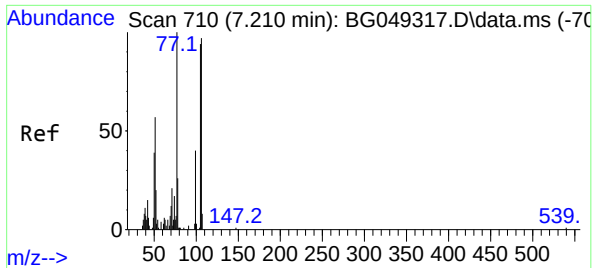

#6
Benzaldehyde
Concen: 2.136 ng/ul
RT: 7.199 min Scan# 708
Delta R.T. -0.013 min
Lab File: BG049322.D
Acq: 13 Jul 2021 20:26

Instrument :
BNA_G
ClientSampleId :
C0AW8

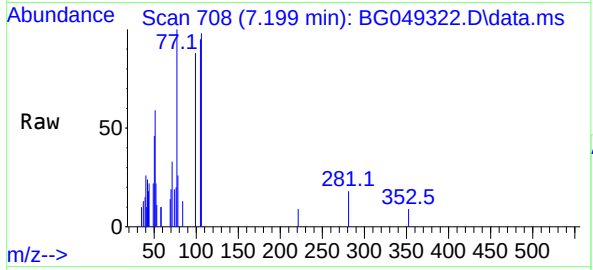

Tgt Ion: 77 Resp: 3170

Ion	Ratio	Lower	Upper
77	100		
105	94.6	72.6	109.0
106	98.4	72.3	108.5

