

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
 Data File : BG049315.D
 Acq On : 13 Jul 2021 12:13
 Operator : CG/JU
 Sample : PB137519BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK519

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049315.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.108	6	12	18	rBV4	24005	51112	4.87%	0.488%
2	3.466	67	73	77	rVB4	8266	15682	1.50%	0.150%
3	3.566	88	90	94	rVB4	2465	1824	0.17%	0.017%
4	3.666	106	107	111	rVB3	2941	2311	0.22%	0.022%
5	3.877	139	143	159	rBV	108857	208800	19.91%	1.993%
6	4.065	173	175	177	rVB2	2497	1837	0.18%	0.018%
7	4.118	183	184	186	rBV2	2345	1468	0.14%	0.014%
8	4.588	261	264	266	rBV3	1497	1506	0.14%	0.014%
9	4.735	286	289	291	rVB3	2425	2378	0.23%	0.023%
10	4.753	291	292	295	rBV3	2014	1890	0.18%	0.018%
11	4.812	300	302	304	rBV3	1416	1489	0.14%	0.014%
12	5.393	399	401	404	rBV	1548	1433	0.14%	0.014%
13	5.869	478	482	483	rBV3	1236	1555	0.15%	0.015%
14	6.592	602	605	609	rVB2	1197	1800	0.17%	0.017%
15	6.850	644	649	650	rBB3	1162	1483	0.14%	0.014%
16	6.915	658	660	664	rBV2	1101	1622	0.15%	0.015%
17	6.968	664	669	671	rBV3	1007	1802	0.17%	0.017%
18	7.221	706	712	721	rBV	162816	289736	27.63%	2.765%
19	7.385	732	740	751	rBV	101357	173953	16.59%	1.660%
20	7.597	769	776	789	rVB	159058	278125	26.52%	2.655%
21	8.067	848	856	862	rBV	100969	171971	16.40%	1.641%
22	8.178	870	875	877	rBV2	1627	2145	0.20%	0.020%
23	8.772	969	976	987	rBV2	197849	347048	33.10%	3.312%
24	9.236	1047	1055	1065	rVB	158195	282070	26.90%	2.692%
25	9.383	1075	1080	1082	rBV	923	1579	0.15%	0.015%
26	9.959	1168	1178	1188	rVB2	143153	262467	25.03%	2.505%
27	10.505	1264	1271	1281	rBV	204240	376060	35.86%	3.589%
28	10.646	1291	1295	1298	rVB	1829	1649	0.16%	0.016%
29	10.887	1330	1336	1344	rVB	135324	236262	22.53%	2.255%
30	11.022	1351	1359	1369	rBV	185712	350503	33.43%	3.345%
31	12.473	1600	1606	1612	rBV2	3117	5283	0.50%	0.050%
32	12.655	1634	1637	1643	rBV	752	1384	0.13%	0.013%
33	13.419	1763	1767	1770	rBV2	1134	1395	0.13%	0.013%
34	13.778	1825	1828	1831	rVB2	1198	1426	0.14%	0.014%
35	14.113	1877	1885	1894	rBV	398750	583619	55.66%	5.570%
36	14.406	1928	1935	1946	rVB	397123	631594	60.23%	6.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
 Data File : BG049315.D
 Acq On : 13 Jul 2021 12:13
 Operator : CG/JU
 Sample : PB137519BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK519

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

37	14.712	1978	1987	1995	rBV	220620	349562	33.34%	3.336%
38	14.906	2012	2020	2030	rBV	172256	300753	28.68%	2.871%
39	15.705	2149	2156	2163	rBV	523247	778820	74.27%	7.433%
40	15.816	2170	2175	2189	rBV	136050	232805	22.20%	2.222%
41	15.946	2192	2197	2201	rVB4	6763	11900	1.13%	0.114%
42	16.392	2270	2273	2274	rVB2	1615	1584	0.15%	0.015%
43	16.410	2274	2276	2278	rBV	2118	1547	0.15%	0.015%
44	16.492	2284	2290	2292	rBV	2812	4027	0.38%	0.038%
45	17.209	2407	2412	2413	rVB	1339	1887	0.18%	0.018%
46	17.244	2413	2418	2419	rBV2	1798	1827	0.17%	0.017%
47	17.462	2449	2455	2464	rVB	300269	451730	43.08%	4.312%
48	17.561	2465	2472	2479	rBV	592103	895773	85.43%	8.550%
49	17.738	2498	2502	2505	rBV	1024	1545	0.15%	0.015%
50	17.814	2511	2515	2516	rBV3	1342	1521	0.15%	0.015%
51	17.932	2533	2535	2539	rVB3	1403	1554	0.15%	0.015%
52	18.120	2565	2567	2569	rBV3	1947	1552	0.15%	0.015%
53	18.290	2593	2596	2598	rBV	1294	1684	0.16%	0.016%
54	18.419	2614	2618	2619	rBV	1543	2111	0.20%	0.020%
55	18.842	2688	2690	2694	rBV3	2405	2239	0.21%	0.021%
56	19.001	2713	2717	2719	rBV2	1506	1843	0.18%	0.018%
57	19.165	2743	2745	2747	rBV3	1470	1381	0.13%	0.013%
58	19.248	2756	2759	2762	rVB3	1611	1874	0.18%	0.018%
59	19.330	2771	2773	2776	rBV3	1786	2273	0.22%	0.022%
60	19.483	2794	2799	2804	rBV	8107	12750	1.22%	0.122%
61	19.565	2812	2813	2816	rBV3	1594	1413	0.13%	0.013%
62	19.606	2816	2820	2821	rBV2	2147	1458	0.14%	0.014%
63	19.647	2824	2827	2829	rBV3	2269	2028	0.19%	0.019%
64	19.735	2840	2842	2849	rVB2	7962	8840	0.84%	0.084%
65	19.847	2855	2861	2868	rBV2	716946	1048564	100.00%	10.008%
66	20.076	2898	2900	2903	rBV2	1882	2089	0.20%	0.020%
67	20.164	2911	2915	2917	rBV4	2010	2489	0.24%	0.024%
68	20.311	2936	2940	2943	rBV6	4025	7016	0.67%	0.067%
69	20.335	2943	2944	2945	rBV	4786	2840	0.27%	0.027%
70	20.746	3013	3014	3016	rBV	4664	4374	0.42%	0.042%
71	21.745	3178	3184	3193	rVB2	295037	484596	46.22%	4.625%
72	24.818	3696	3707	3720	rVB	359026	1024404	97.70%	9.777%
73	25.041	3736	3745	3756	rVB2	174838	524360	50.01%	5.005%




Sum of corrected areas: 10477274

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
Data File : BG049315.D
Acq On : 13 Jul 2021 12:13
Operator : CG/JU
Sample : PB137519BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

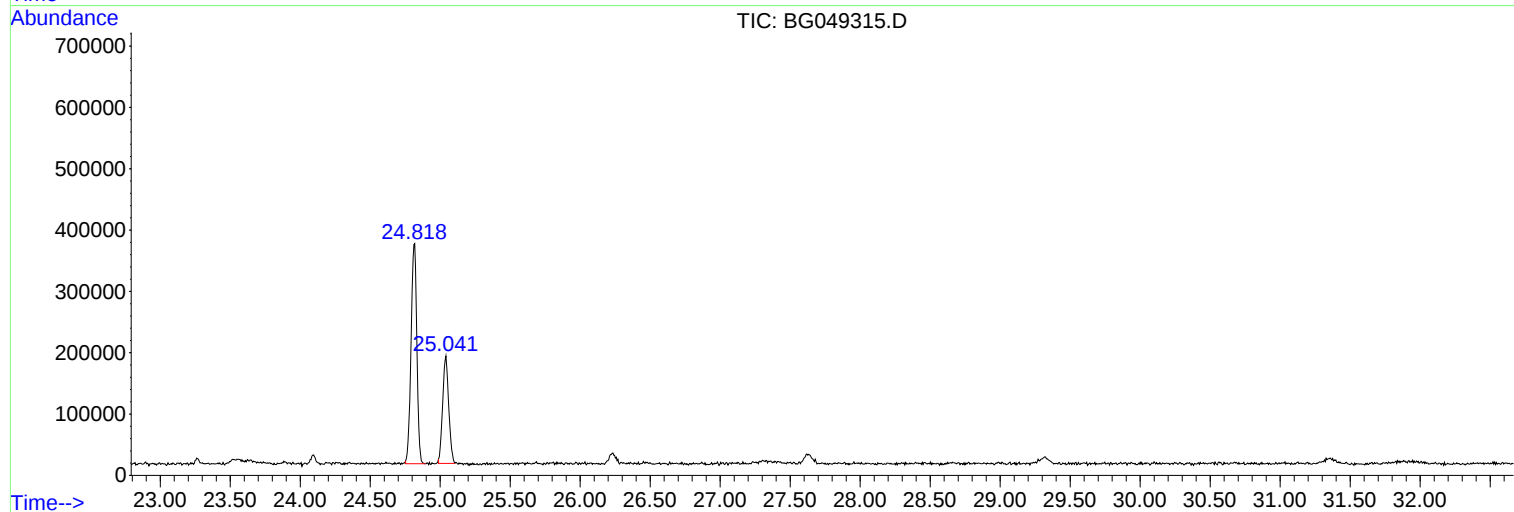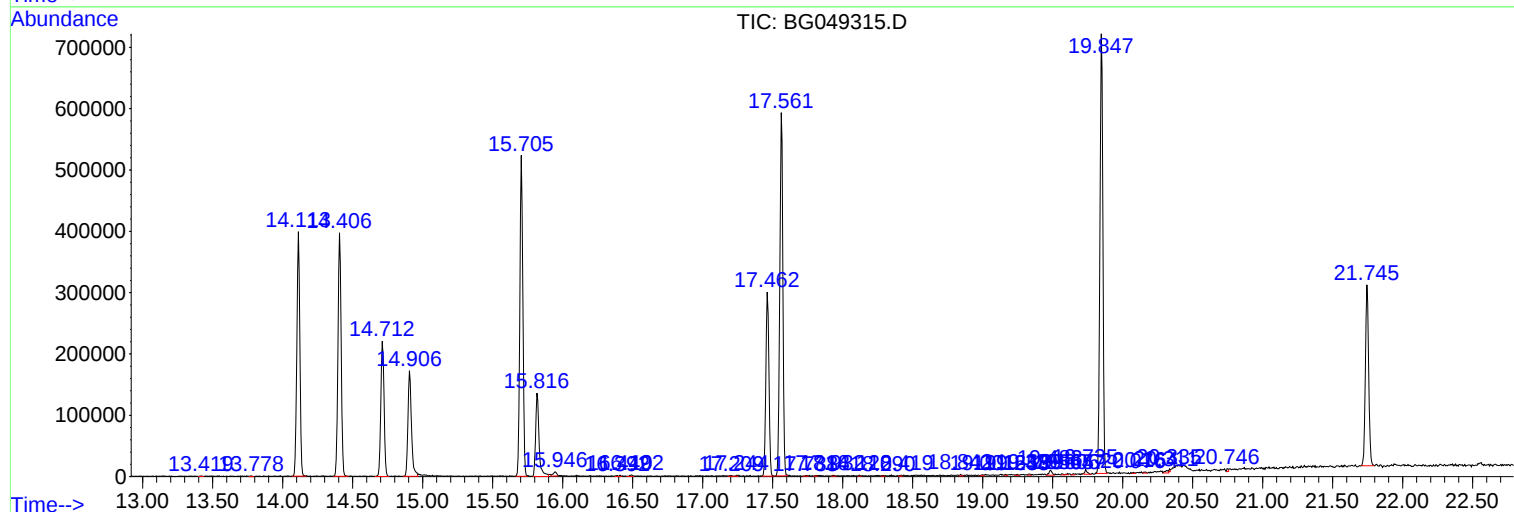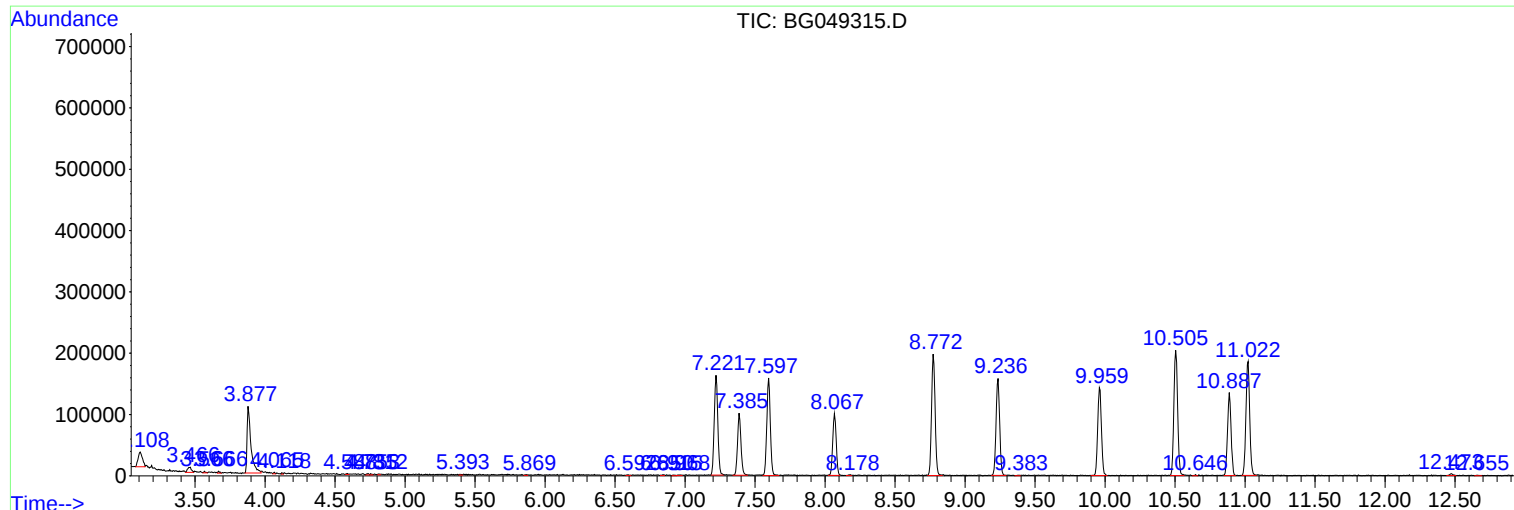

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
Data File : BG049315.D
Acq On : 13 Jul 2021 12:13
Operator : CG/JU
Sample : PB137519BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK519










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.11 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.110	5.94 ng/ul	51112	1,4-Dichlorobenzene-d4	8.067

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	78
2			2-Acetylpiiperidine	127	C7H13NO	097073-22-8	64
3			Cyclohexane	84	C6H12	000110-82-7	52
4			Cyclobutane, ethyl-	84	C6H12	004806-61-5	47
5			Cyclohexane	84	C6H12	000110-82-7	47

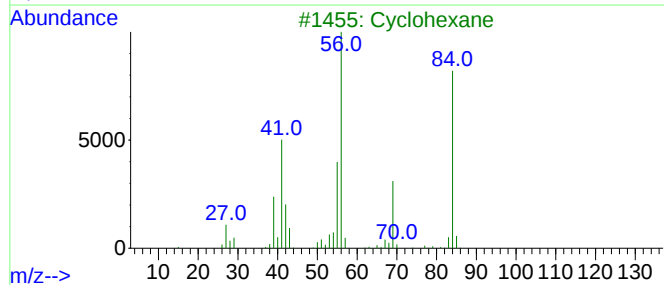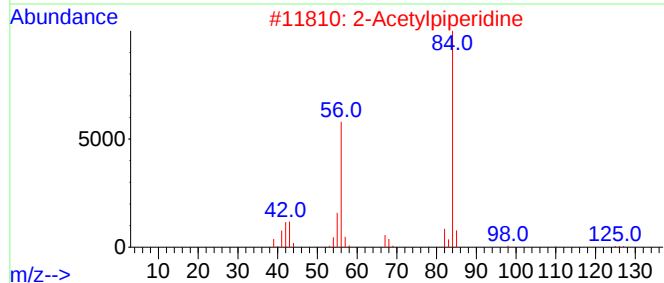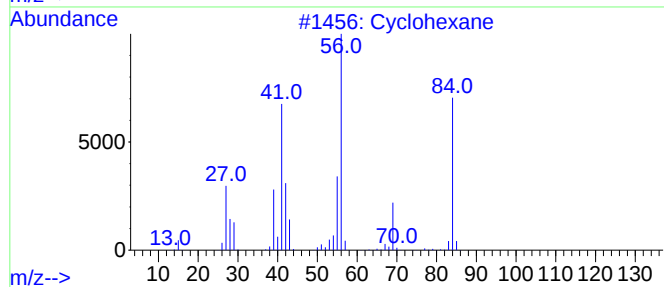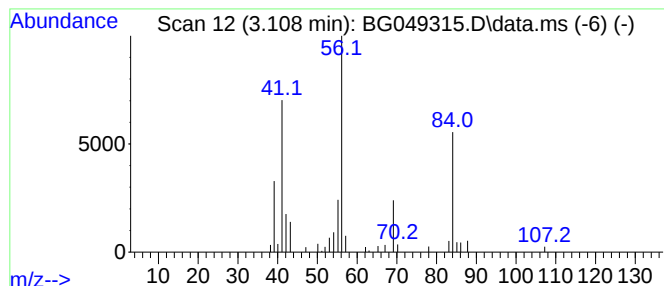

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071221\
Data File : BG049315.D
Acq On : 13 Jul 2021 12:13
Operator : CG/JU
Sample : PB137519BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.110	5.9	ng/ul	51112	1	8.067	171971	20.0