

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017830.D
 Acq On : 13 Jul 2015 19:47
 Operator : TP/UM
 Sample : G2936-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01W3

Quant Time: Jul 14 01:27:56 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 14 01:25:57 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	75123	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	334712	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	195692	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	412012	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	424458	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	401891	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	3140	1.69	ng/uL	0.00
5) Phenol-d5	6.77	99	55059	7.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	132326	31.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	142648	24.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	91397	15.22	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	88361	31.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	84188	29.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	130653	26.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	6365	0.93	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	469960	31.57	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	584801	32.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	19244	6.06	ng/ul	0.00
57) Fluorene-d10	15.24	176	431642	32.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	61759	24.82	ng/ul	0.00
70) Anthracene-d10	17.10	188	624476	32.41	ng/ul	0.00
78) Pyrene-d10	19.40	212	685094	33.48	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	608020	30.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.15	88	6007	3.05	ng/uL#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017830.D
Acq On : 13 Jul 2015 19:47
Operator : TP/UM
Sample : G2936-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01W3

Quant Time: Jul 14 01:27:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 01:25:57 2015
Response via : Initial Calibration

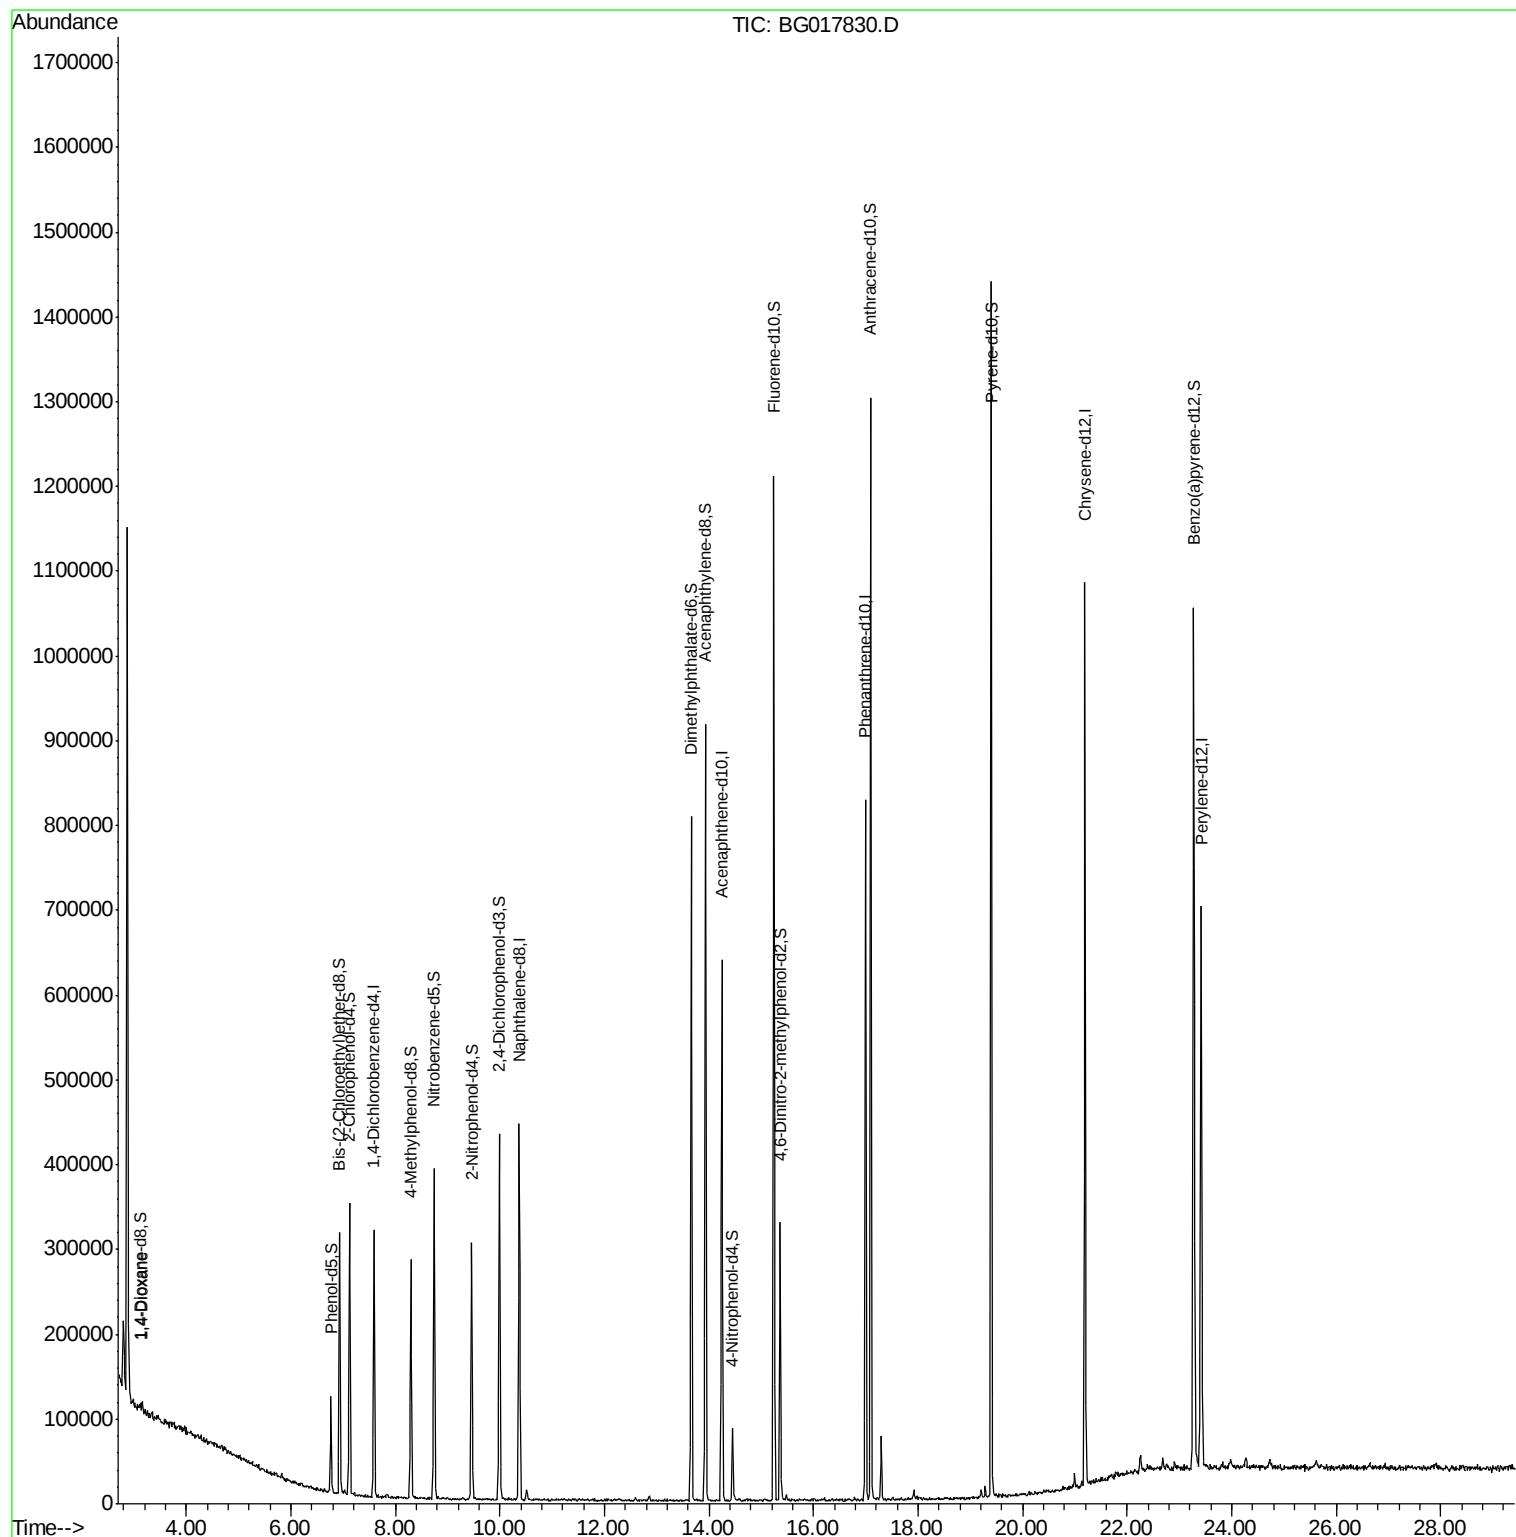

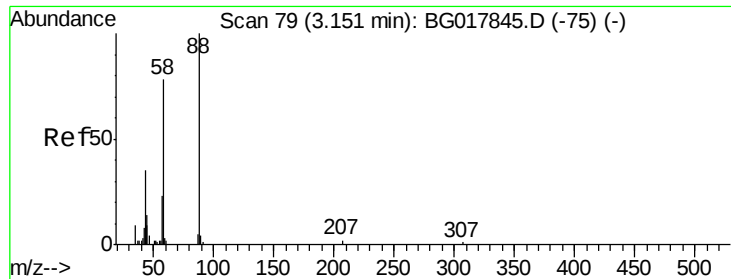

#2
 1,4-Dioxane
 Concen: 3.05 ng/uL
 RT: 3.15 min Scan# 79
 Delta R.T. 0.00 min
 Lab File: BG017830.D
 Acq: 13 Jul 2015 19:47

Instrument :
 BNA_G
 ClientSampleId :
 C01W3

Tgt Ion: 88 Resp: 6007
 Ion Ratio Lower Upper
 88 100
 43 47.9 30.9 46.3#
 58 67.5 61.4 92.2

