

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017841.D
 Acq On : 14 Jul 2015 2:47
 Operator : TP/UM
 Sample : G2936-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01X2

Quant Time: Jul 14 06:33:56 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 14 02:07:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	68906	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	308772	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	179256	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	379662	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	388203	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	374514	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	2353	1.38	ng/uL	0.00
5) Phenol-d5	6.77	99	43841	6.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	117467	30.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	115812	21.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	76524	13.89	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	74660	28.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	66777	25.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	104948	22.96	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	392272	28.77	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	483574	29.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	15565	5.35	ng/ul	0.00
57) Fluorene-d10	15.24	176	371009	30.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	52928	23.08	ng/ul	0.00
70) Anthracene-d10	17.09	188	566274	31.89	ng/ul	0.00
78) Pyrene-d10	19.40	212	635379	33.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	555845	29.75	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.15	88	5144	2.85	ng/uL#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017841.D
Acq On : 14 Jul 2015 2:47
Operator : TP/UM
Sample : G2936-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01X2

Quant Time: Jul 14 06:33:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 02:07:11 2015
Response via : Initial Calibration

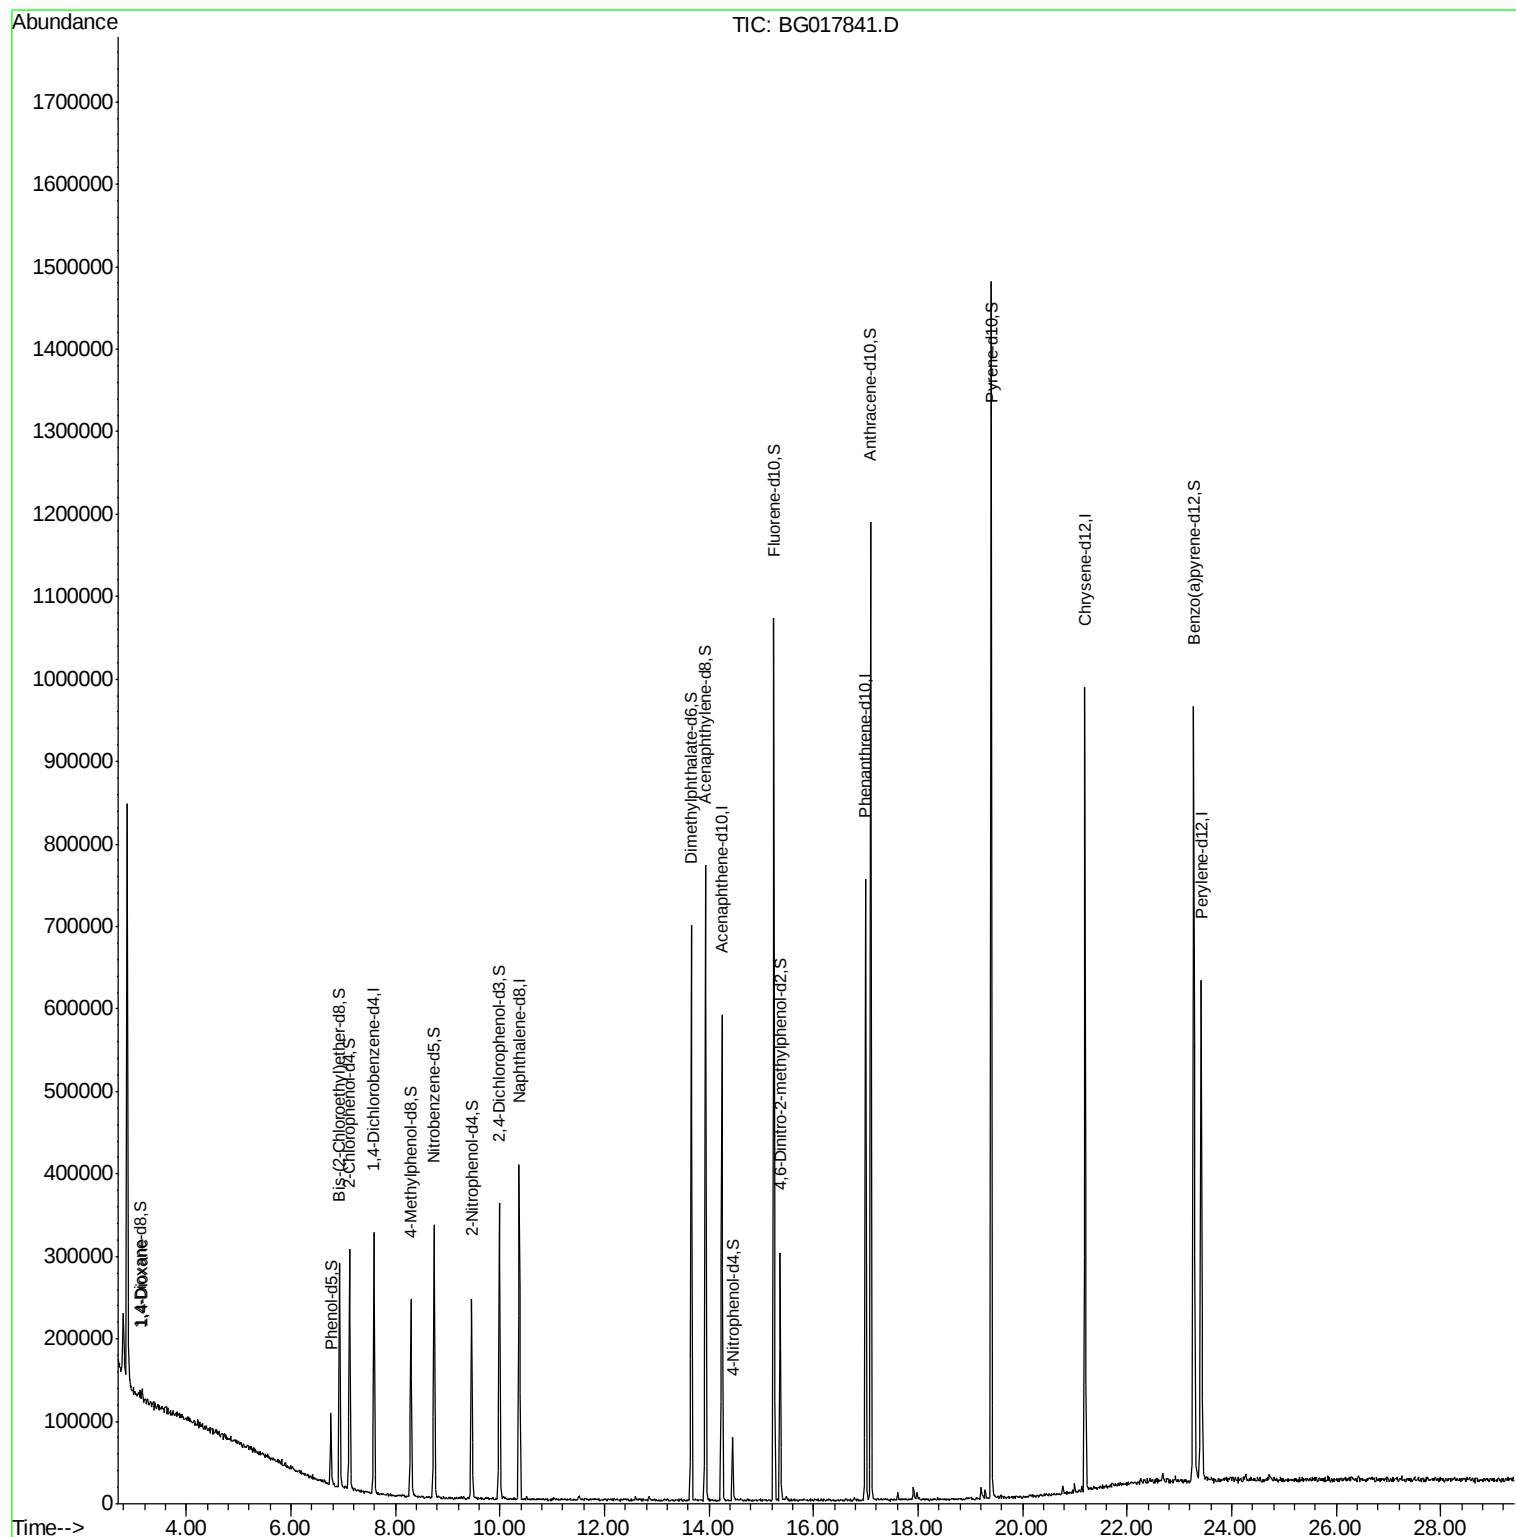

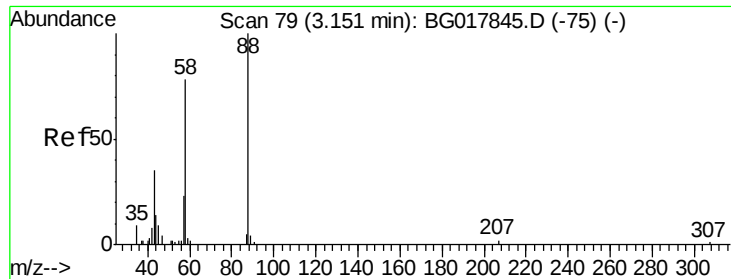

#2
 1,4-Dioxane
 Concen: 2.85 ng/uL
 RT: 3.15 min Scan# 79
 Delta R.T. -0.00 min
 Lab File: BG017841.D
 Acq: 14 Jul 2015 2:47

Instrument :
 BNA_G
 ClientSampleId :
 C01X2

Tgt Ion: 88 Resp: 5144
 Ion Ratio Lower Upper
 88 100
 43 47.0 30.9 46.3#
 58 79.9 61.4 92.2

