

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017847.D
 Acq On : 14 Jul 2015 6:51
 Operator : TP/UM
 Sample : G2938-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0204

Quant Time: Jul 14 07:34:07 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 14 07:26:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	68035	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	306668	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	173890	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	363668	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	362886	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	340725	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	2830	1.68	ng/uL	0.00
5) Phenol-d5	6.77	99	46371	7.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	137331	35.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	131416	25.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	81512	14.99	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	84079	32.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	72821	28.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	117392	25.86	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.66	166	440805	33.33	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	565610	35.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	12434	4.41	ng/ul	0.00
57) Fluorene-d10	15.25	176	414791	35.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	53469	24.35	ng/ul	0.00
70) Anthracene-d10	17.10	188	614625	36.14	ng/ul	0.00
78) Pyrene-d10	19.41	212	664001	37.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	577151	33.96	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.15	88	11393	6.39 ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017847.D
Acq On : 14 Jul 2015 6:51
Operator : TP/UM
Sample : G2938-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0204

Quant Time: Jul 14 07:34:07 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 07:26:48 2015
Response via : Initial Calibration

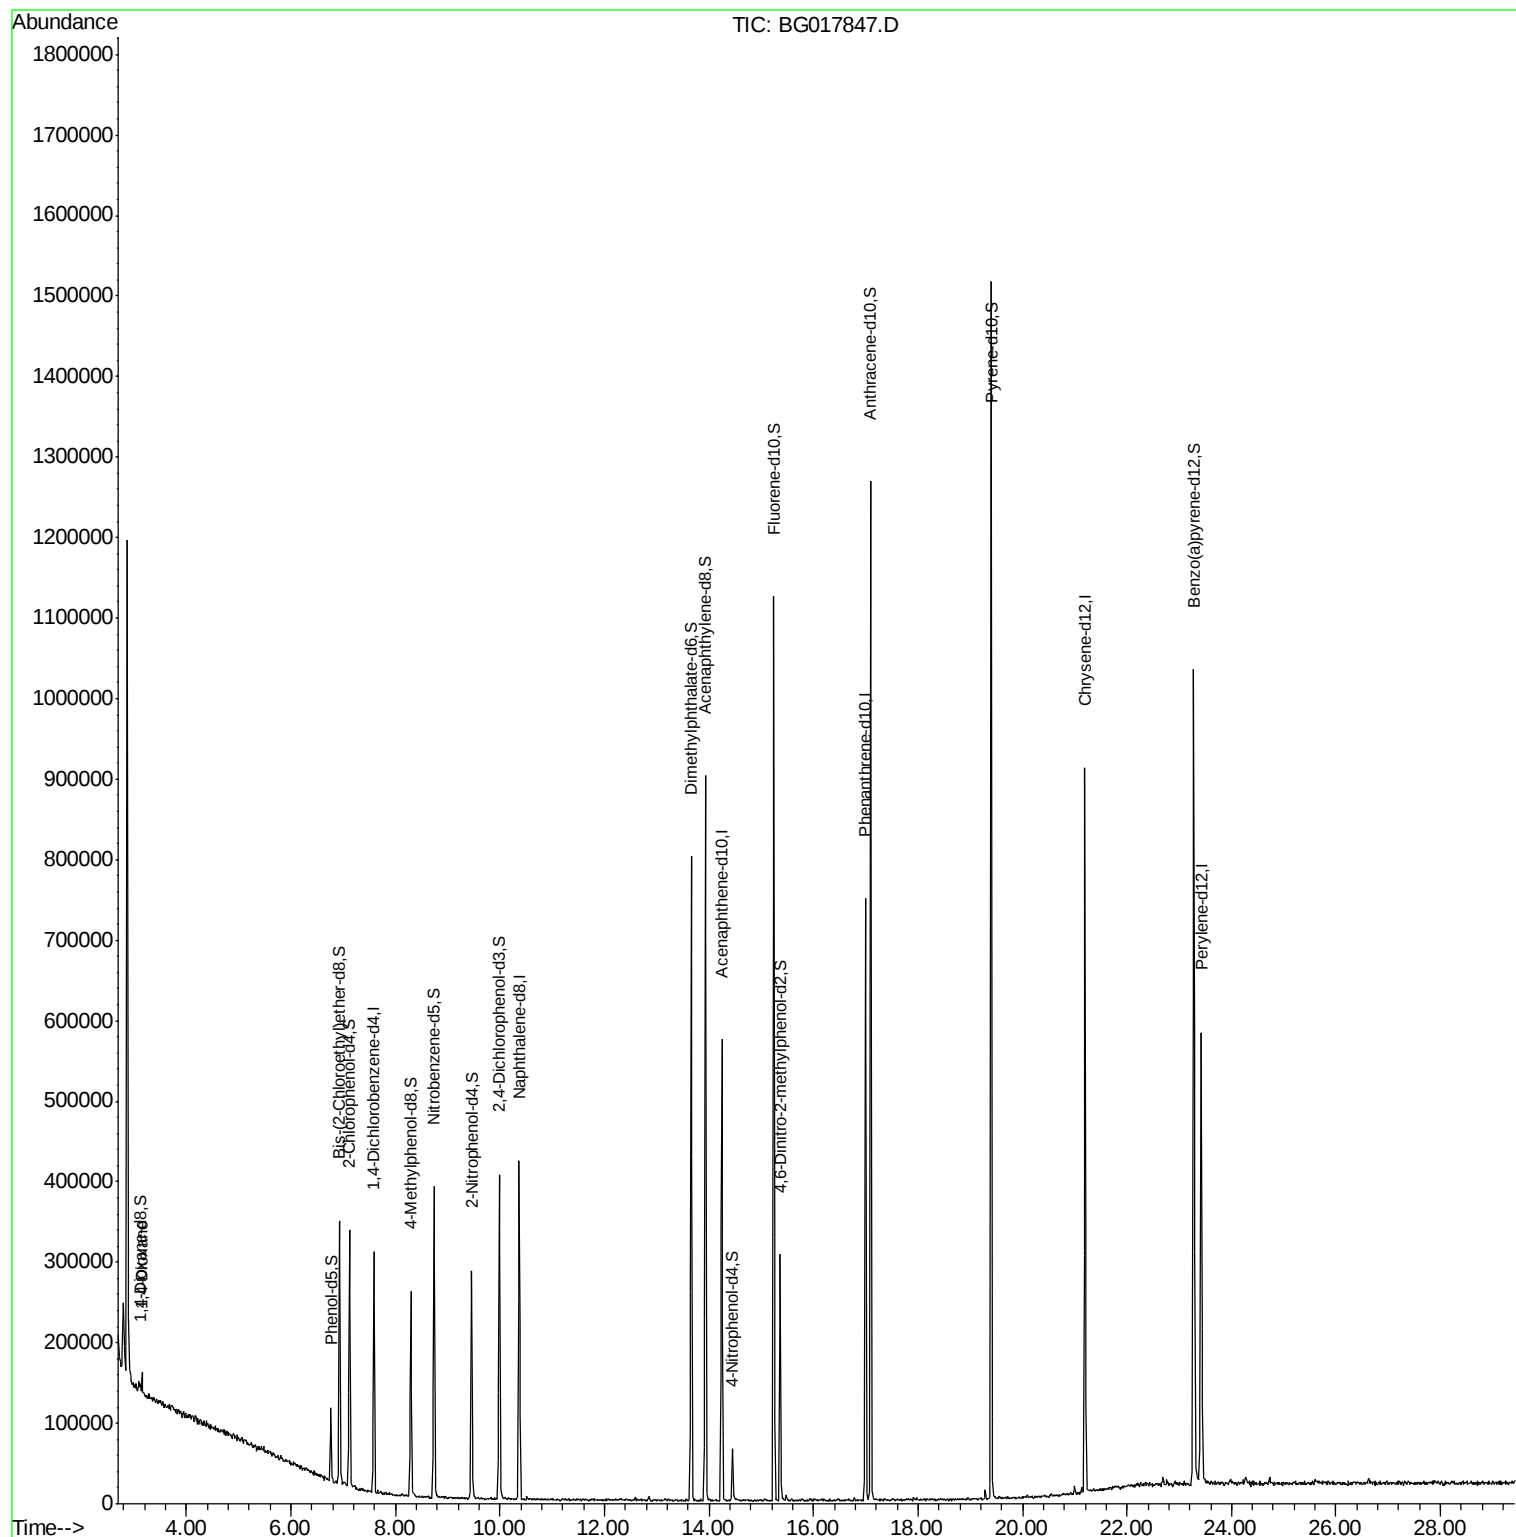

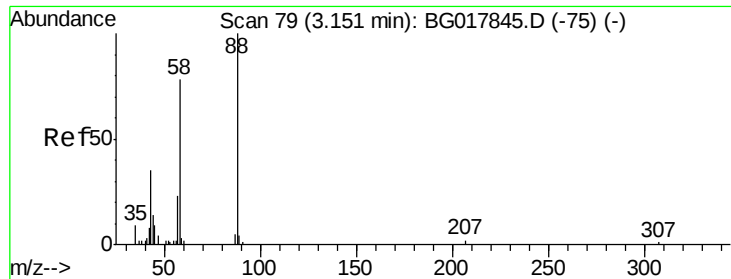

#2
 1,4-Dioxane
 Concen: 6.39 ng/uL
 RT: 3.15 min Scan# 79
 Delta R.T. 0.00 min
 Lab File: BG017847.D
 Acq: 14 Jul 2015 6:51

Instrument :
 BNA_G
 ClientSampleId :
 C0204

Tgt Ion: 88 Resp: 11393
 Ion Ratio Lower Upper
 88 100
 43 45.6 30.9 46.3
 58 79.0 61.4 92.2

