

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017849.D
 Acq On : 14 Jul 2015 8:01
 Operator : TP/UM
 Sample : G2938-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0206

Quant Time: Jul 15 04:46:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 04:02:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	70808	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	328028	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	188471	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	397079	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	407281	20.00	ng/ul	0.00
85) Perylene-d12	23.41	264	383055	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	3284	1.87	ng/uL	0.00
5) Phenol-d5	6.76	99	49081	7.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	121841	30.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	121005	22.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	81238	14.35	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	73924	26.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	63048	22.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	104165	21.45	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.66	166	391227	27.29	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	499908	28.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	14598	4.78	ng/ul	0.00
57) Fluorene-d10	15.24	176	363933	28.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	44672	18.63	ng/ul	0.00
70) Anthracene-d10	17.10	188	537667	28.95	ng/ul	0.00
78) Pyrene-d10	19.40	212	597820	30.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	518275	27.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.16	88	8903	4.79	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017849.D
Acq On : 14 Jul 2015 8:01
Operator : TP/UM
Sample : G2938-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0206

Quant Time: Jul 15 04:46:21 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 04:02:40 2015
Response via : Initial Calibration

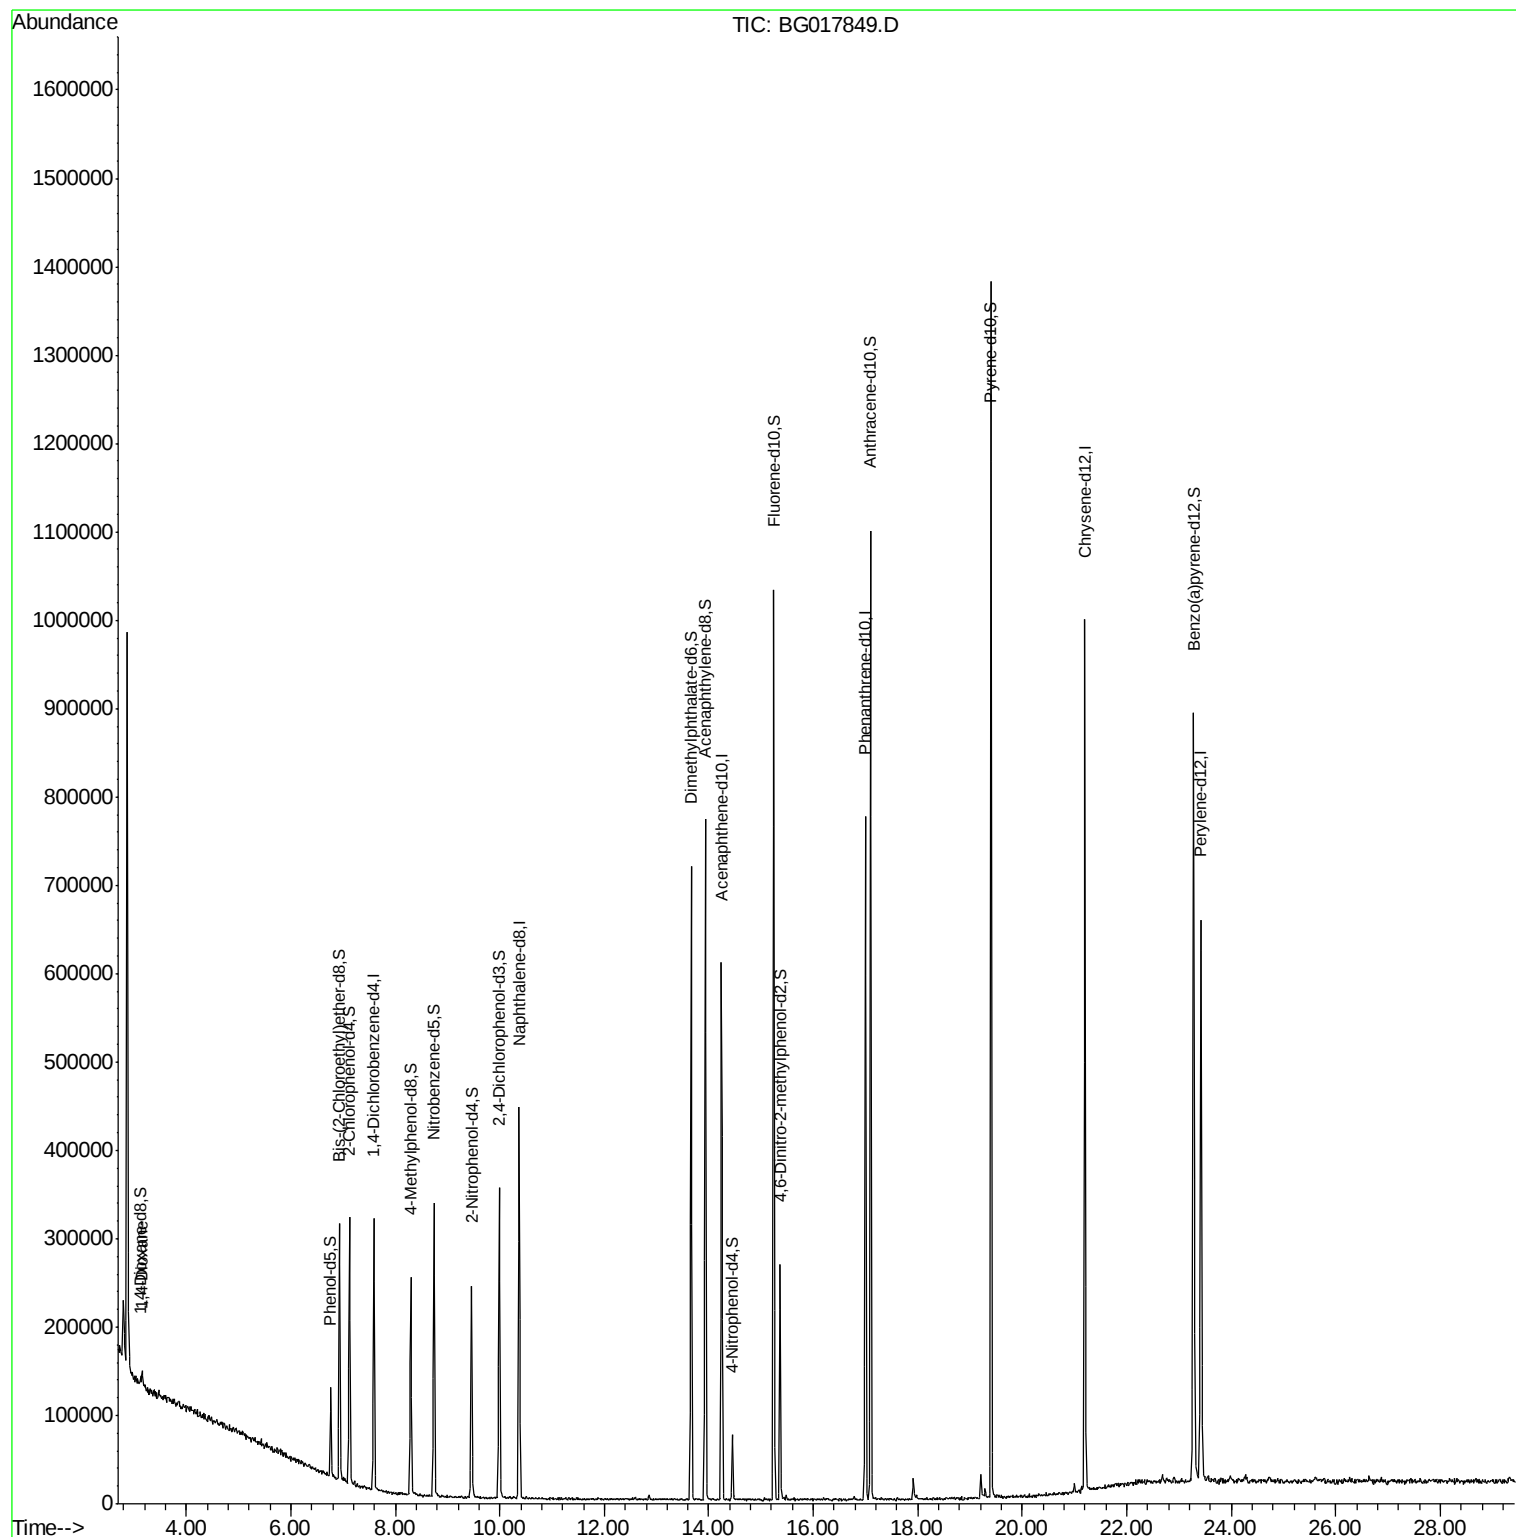

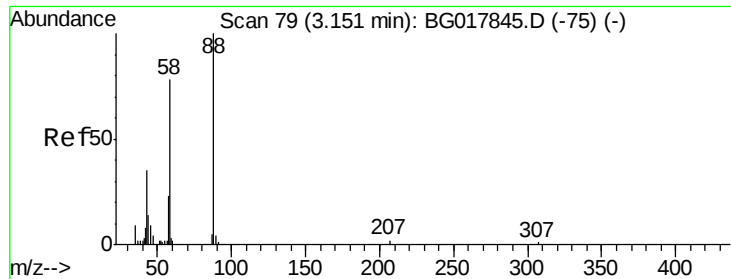

#2
 1,4-Dioxane
 Concen: 4.79 ng/uL
 RT: 3.16 min Scan# 80
 Delta R.T. 0.01 min
 Lab File: BG017849.D
 Acq: 14 Jul 2015 8:01

Instrument :
 BNA_G
 ClientSampleId :
 C0206

Tgt Ion: 88 Resp: 8903
 Ion Ratio Lower Upper
 88 100
 43 42.1 30.9 46.3
 58 73.9 61.4 92.2

