

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017850.D
 Acq On : 14 Jul 2015 8:35
 Operator : TP/UM
 Sample : G2938-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0207

Quant Time: Jul 15 04:04:02 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 04:02:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	63052	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	289735	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	169071	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	353424	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	365004	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	345853	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	2059	1.32	ng/uL	0.00
5) Phenol-d5	6.77	99	37260	6.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	111524	31.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	104100	21.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	64390	12.78	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	66894	27.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	58733	23.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	92256	21.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	3869	0.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	338952	26.36	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	445455	28.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	10598	3.87	ng/ul	0.00
57) Fluorene-d10	15.24	176	325655	28.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	39790	18.64	ng/ul	0.00
70) Anthracene-d10	17.10	188	496125	30.02	ng/ul	0.00
78) Pyrene-d10	19.41	212	555455	31.56	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	487983	28.28	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
83) Bis(2-ethylhexyl)phthalate	21.13	149	18227	1.25	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017850.D
Acq On : 14 Jul 2015 8:35
Operator : TP/UM
Sample : G2938-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0207

Quant Time: Jul 15 04:04:02 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 04:02:40 2015
Response via : Initial Calibration

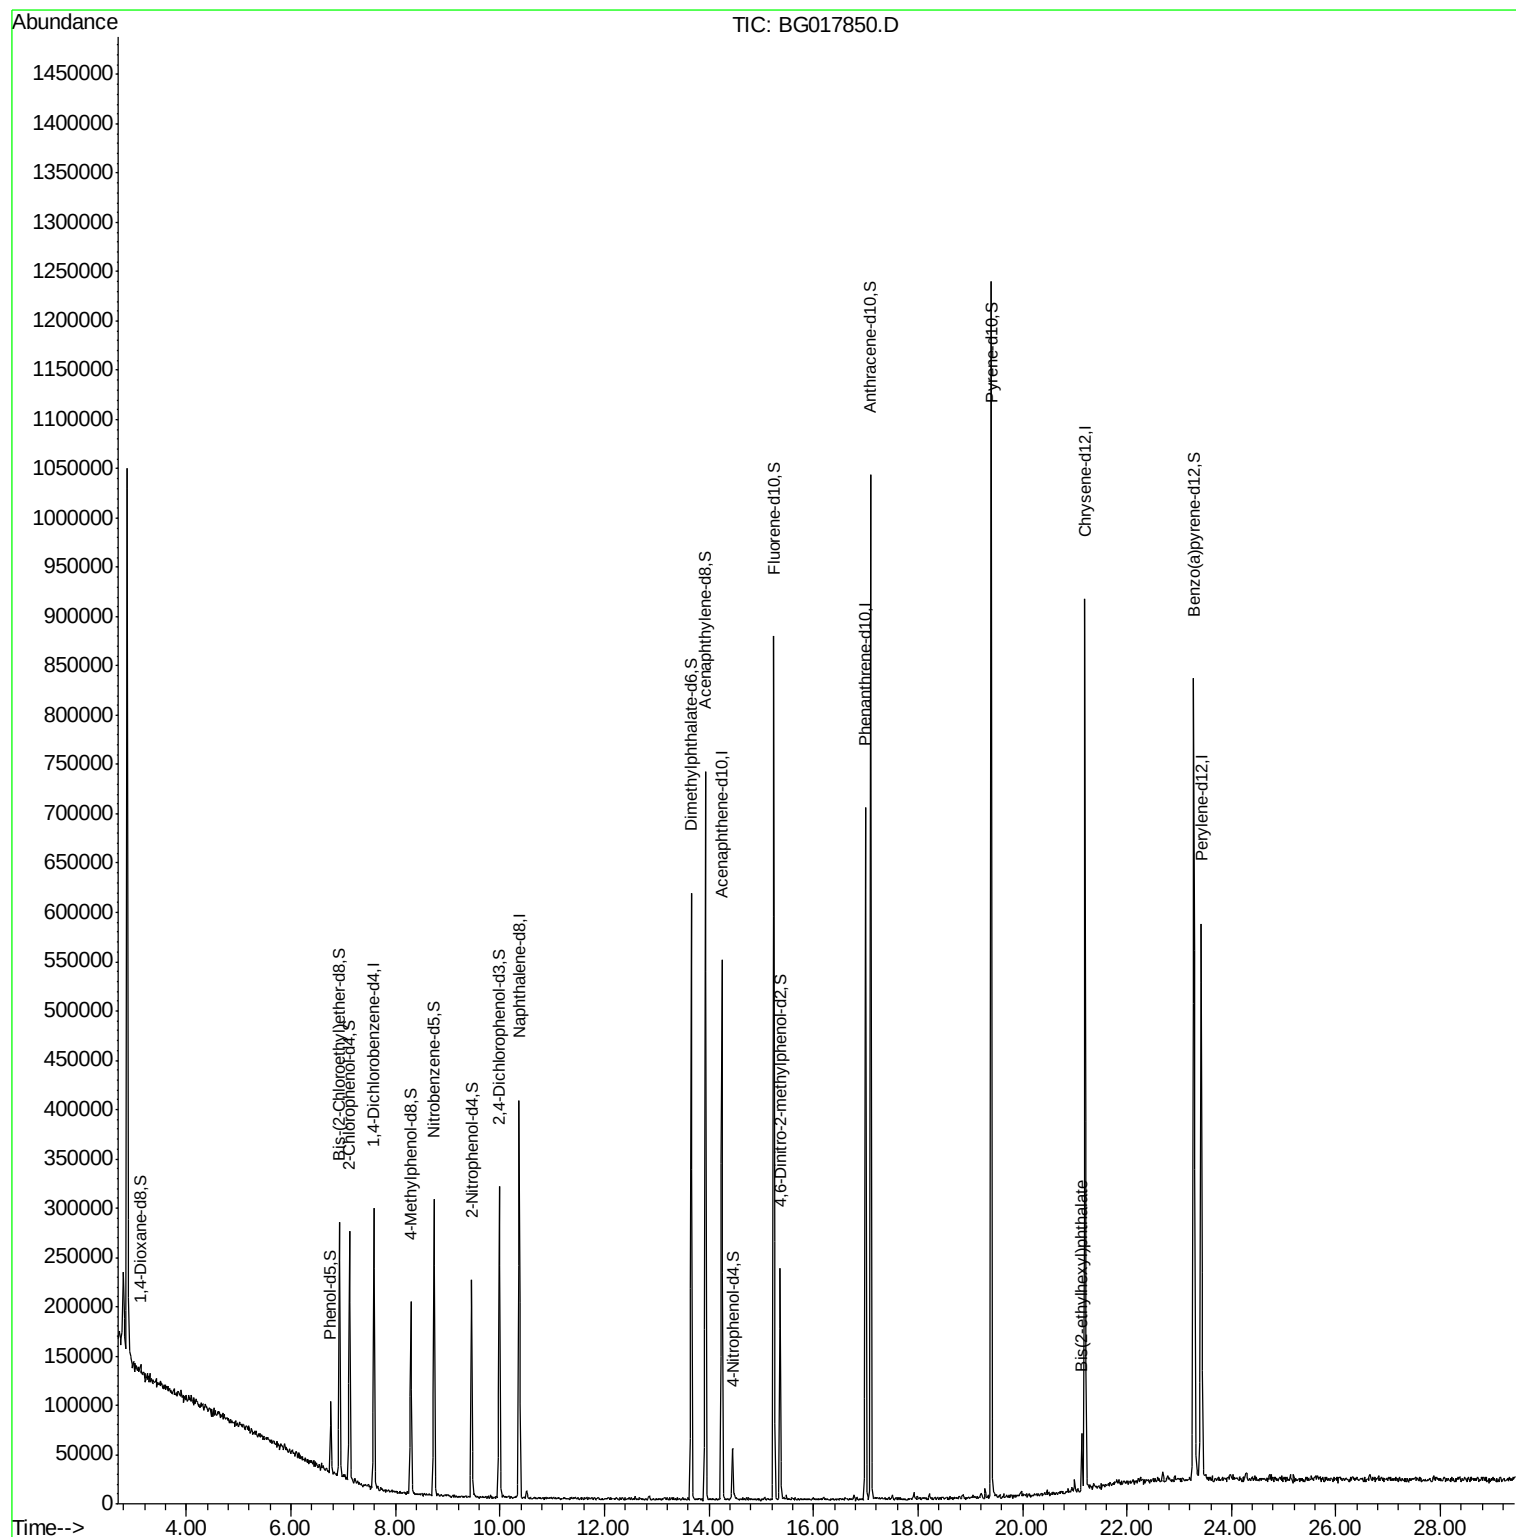

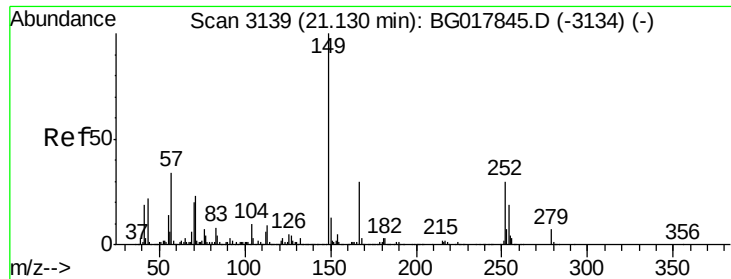

#83

Bis(2-ethylhexyl)phthalate

Concen: 1.25 ng/ul

RT: 21.13 min Scan# 3139

Delta R.T. 0.00 min

Lab File: BG017850.D

Acq: 14 Jul 2015 8:35

Instrument :

BNA_G

ClientSampleId :

C0207


Tgt Ion:149 Resp: 18227

Ion Ratio Lower Upper

149 100

167 32.4 24.9 37.3

279 6.4 6.2 9.2

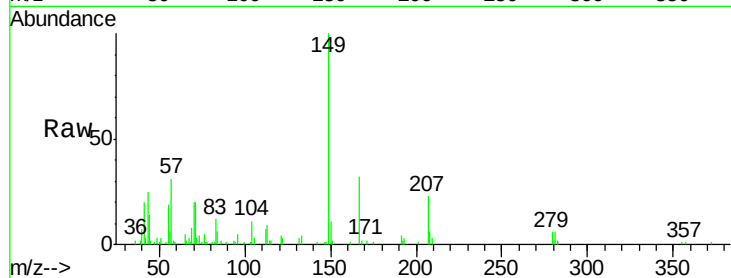

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

