

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
 Data File : BG017854.D
 Acq On : 14 Jul 2015 11:05
 Operator : TP/UM
 Sample : G2938-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01X7

Quant Time: Jul 15 04:04:45 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 04:02:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	68172	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	303355	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.24	164	173816	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	367580	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	372234	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	356173	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	2558	1.51	ng/uL	0.00
5) Phenol-d5	6.76	99	37396	5.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	108221	28.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	102271	19.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	63629	11.68	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	66650	26.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	55487	21.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	88766	19.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	8536	1.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	344806	26.08	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	443223	27.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	9831	3.49	ng/ul	-0.01
57) Fluorene-d10	15.24	176	322195	27.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	37827	17.04	ng/ul	0.00
70) Anthracene-d10	17.09	188	488261	28.40	ng/ul	0.00
78) Pyrene-d10	19.40	212	534960	29.81	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	445909	25.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.15	88	9216	5.16	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071315\
Data File : BG017854.D
Acq On : 14 Jul 2015 11:05
Operator : TP/UM
Sample : G2938-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01X7

Quant Time: Jul 15 04:04:45 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 04:02:40 2015
Response via : Initial Calibration

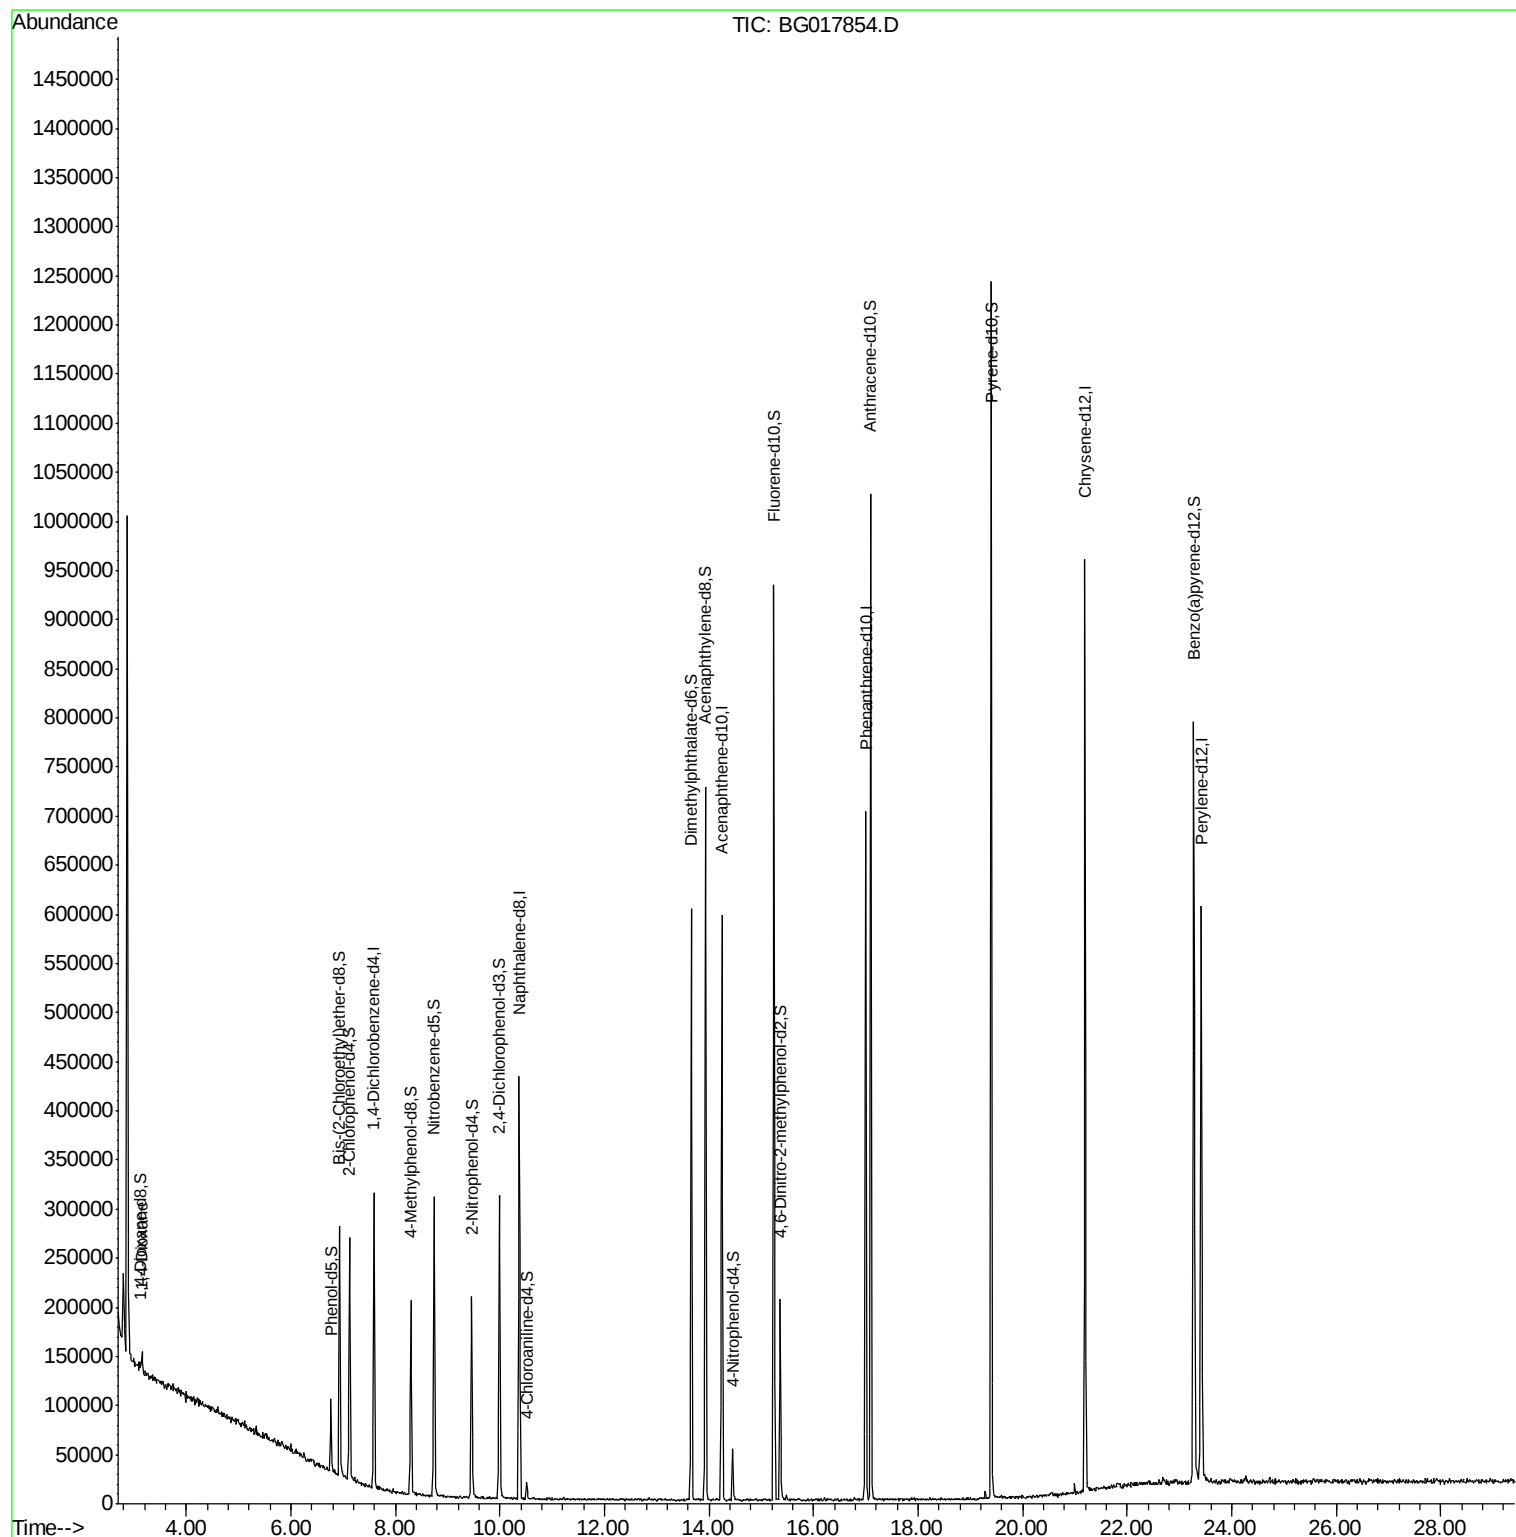

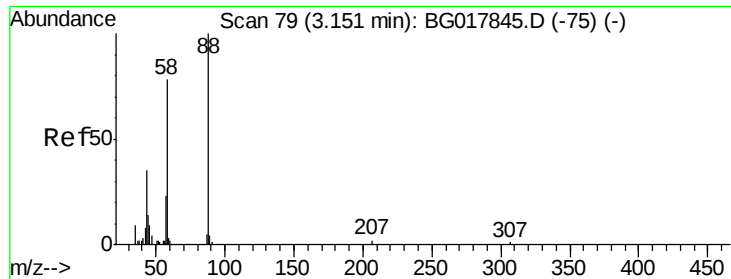

#2
 1,4-Dioxane
 Concen: 5.16 ng/uL
 RT: 3.15 min Scan# 79
 Delta R.T. 0.00 min
 Lab File: BG017854.D
 Acq: 14 Jul 2015 11:05

Instrument :
 BNA_G
 ClientSampleId :
 C01X7

Tgt Ion: 88 Resp: 9216
 Ion Ratio Lower Upper
 88 100
 43 43.8 30.9 46.3
 58 87.1 61.4 92.2

