
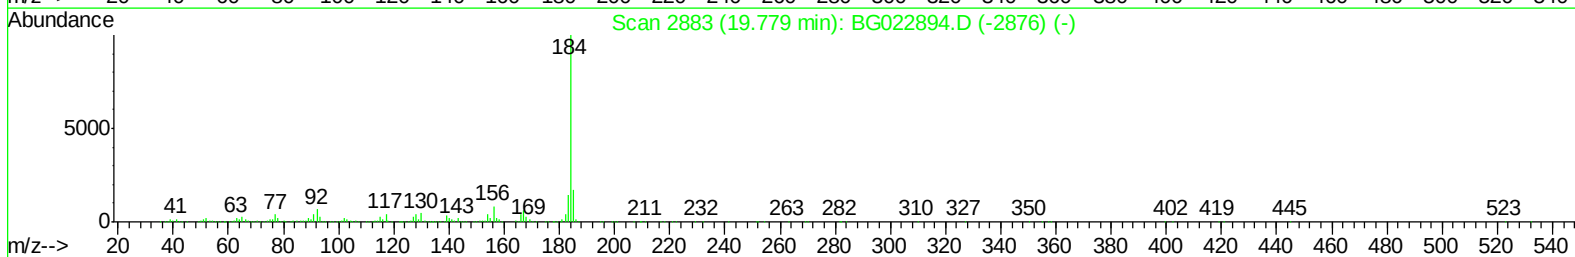
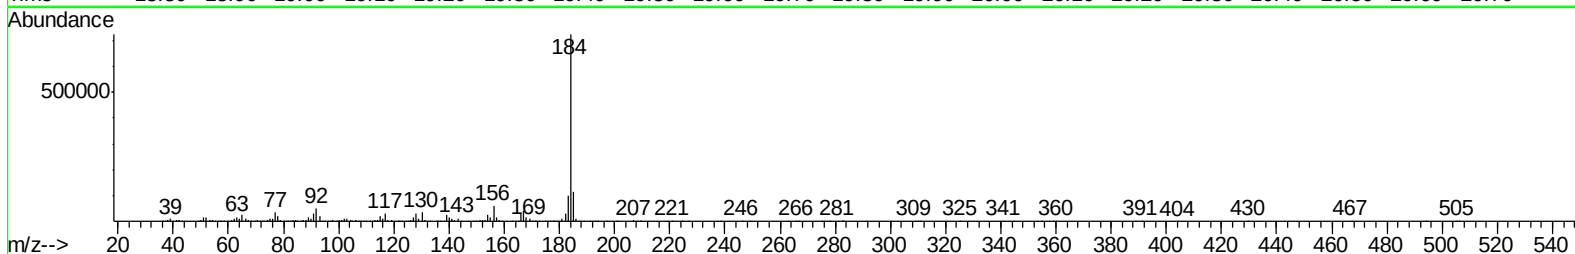


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071316\
Data File : BG023081.D
Acq On : 13 Jul 2016 23:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 08:00:10 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

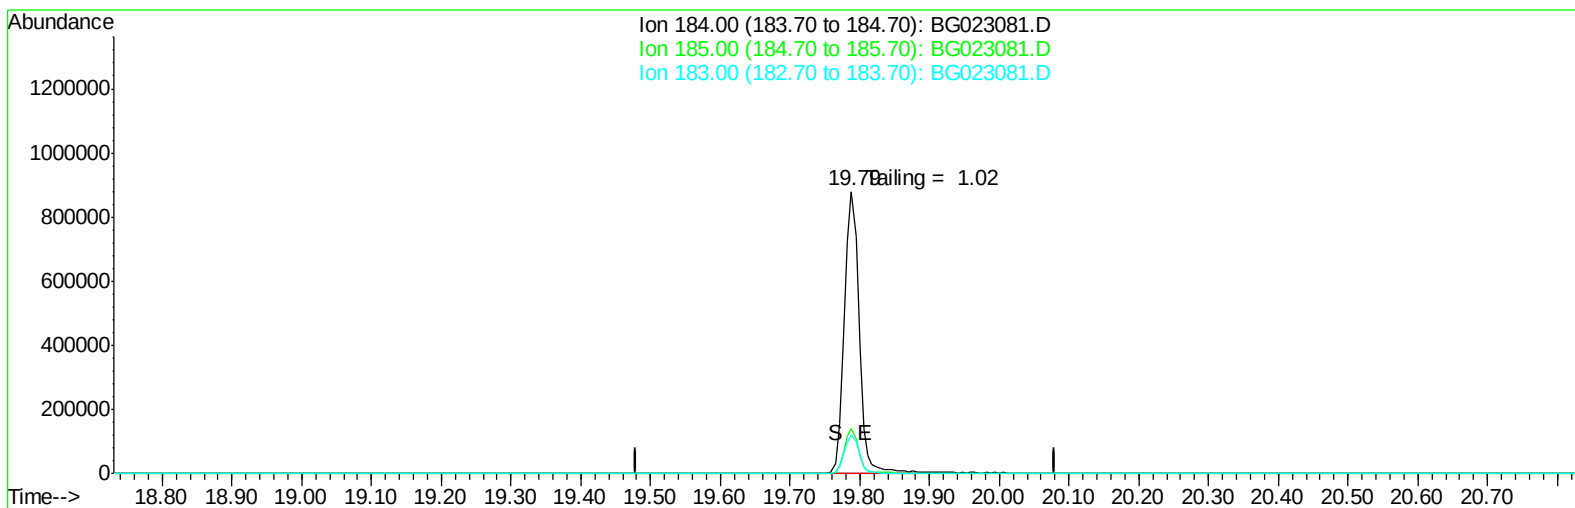

TIC: BG023081.D

(76) Benzidine




19.779min (-19.779) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.80	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071316\
Data File : BG023081.D
Acq On : 13 Jul 2016 23:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 08:00:10 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

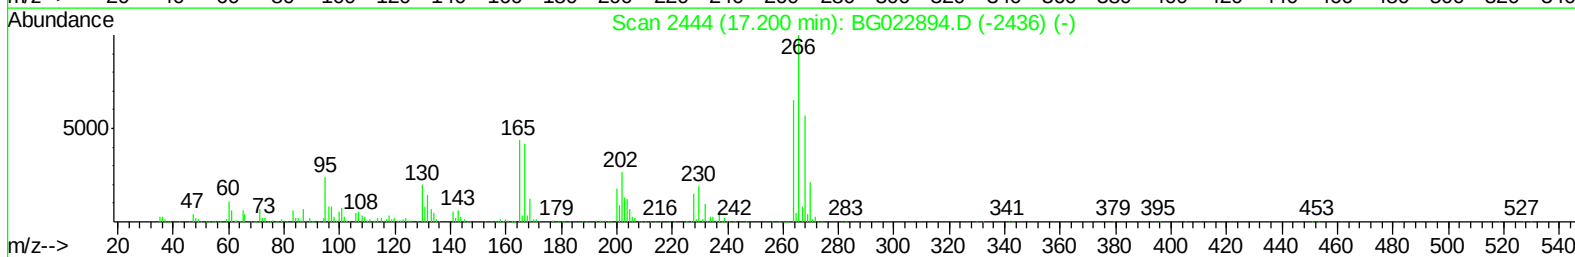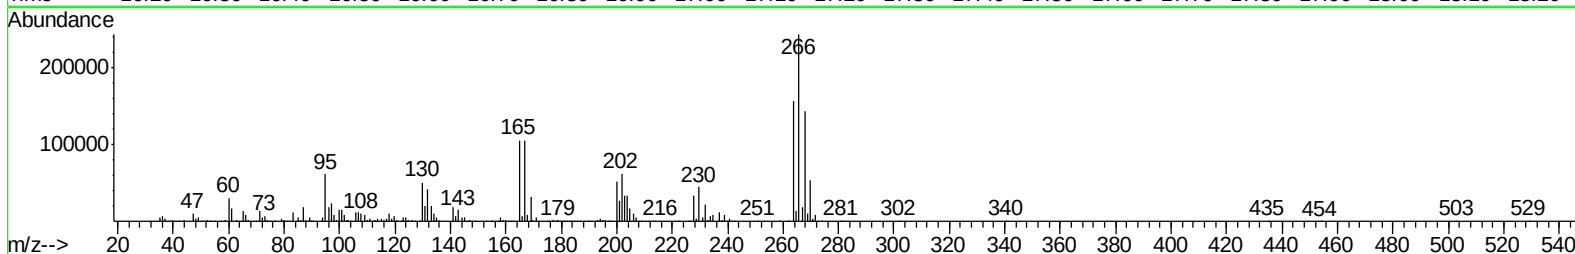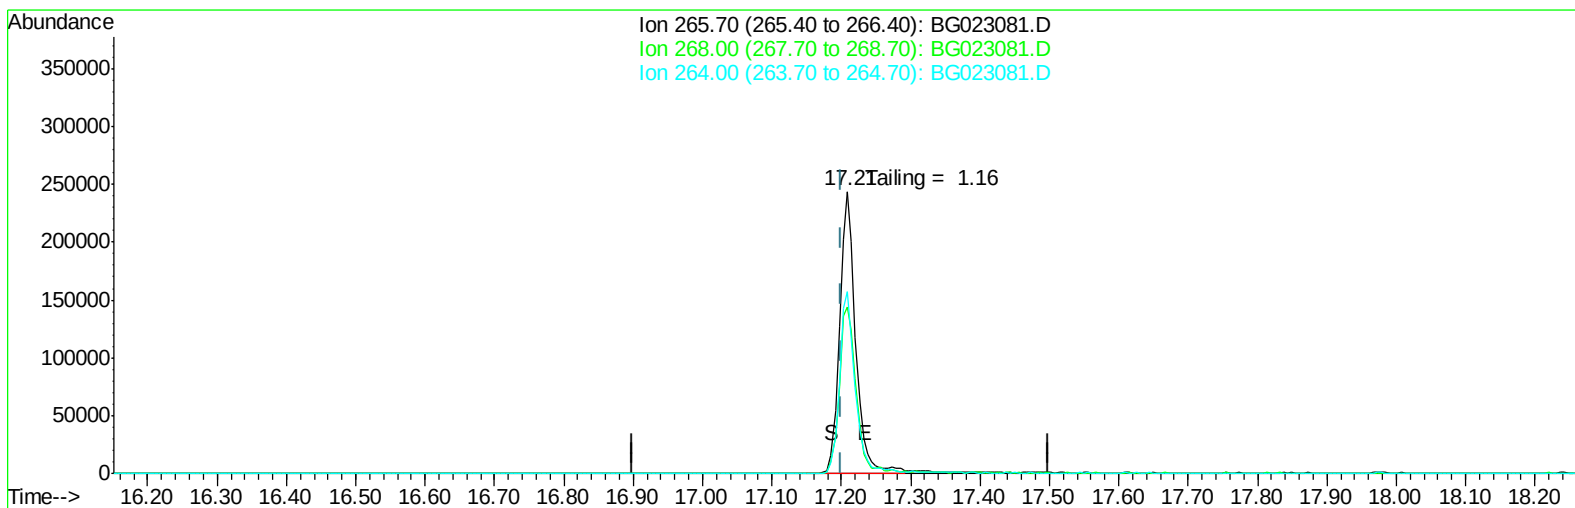

TIC: BG023081.D

(69) Pentachlorophenol (C)

17.209min (+0.009) 305387.31ng

response 299347

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.25
264.00	63.20	64.42
0.00	0.00	0.00