


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071316\
 Data File : BG023067.D
 Acq On : 13 Jul 2016 13:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

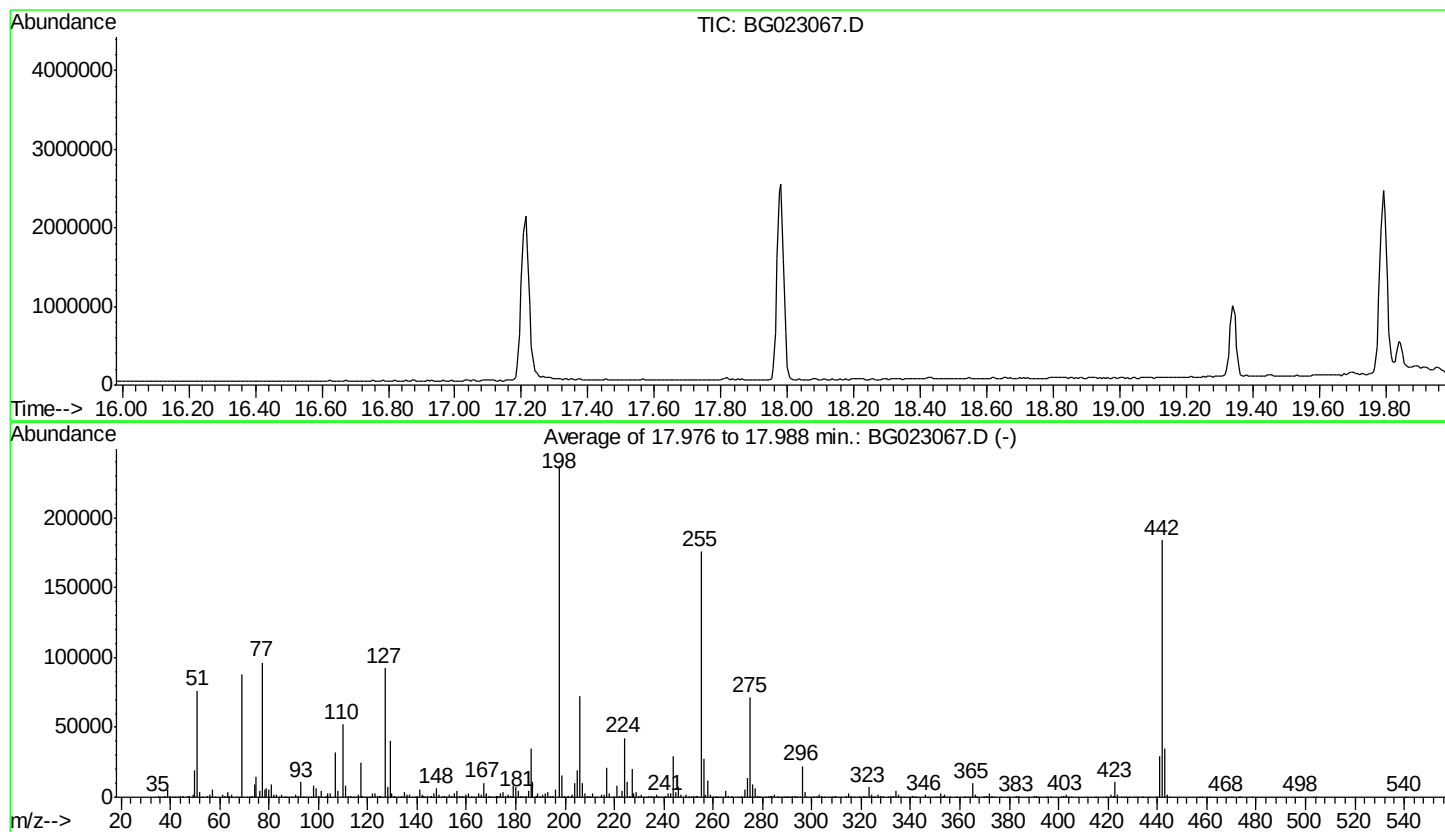

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	76323	PASS
68	69	0.00	2	0.3	240	PASS
69	198	0.00	100	37.1	88081	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.0	92488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	237226	PASS
199	198	5	9	6.7	15797	PASS
275	198	10	60	30.1	71290	PASS
365	198	1	100	4.1	9670	PASS
441	442	0.01	24	15.8	29141	PASS
442	198	50	100	77.6	184042	PASS
443	442	15	24	19.1	35064	PASS