


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071316\
 Data File : BG023081.D
 Acq On : 13 Jul 2016 23:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

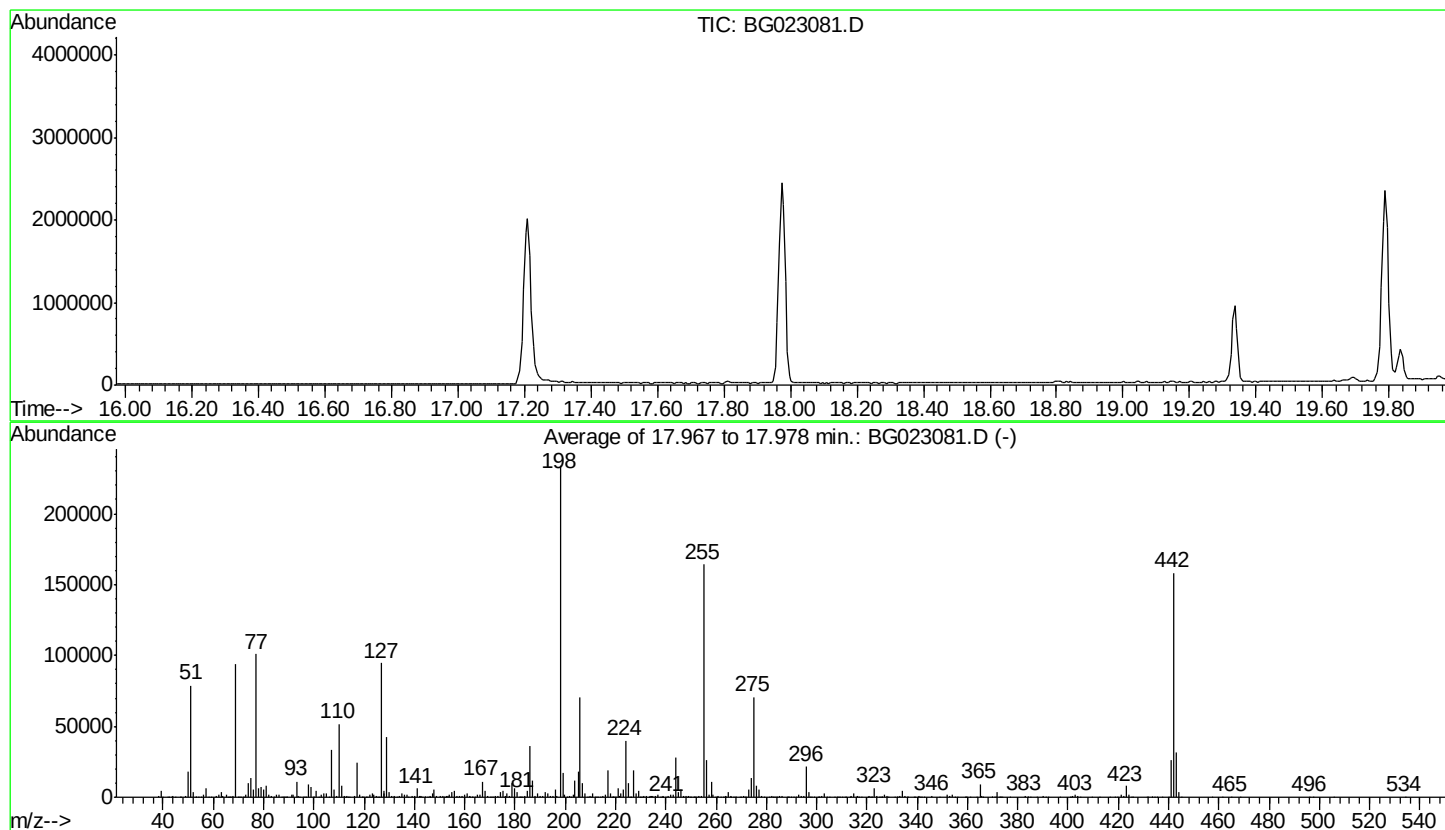

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	78967	PASS
68	69	0.00	2	0.8	795	PASS
69	198	0.00	100	40.2	93931	PASS
70	69	0.00	2	0.4	332	PASS
127	198	10	80	40.5	94722	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233920	PASS
199	198	5	9	7.2	16879	PASS
275	198	10	60	30.3	70773	PASS
365	198	1	100	4.0	9268	PASS
441	442	0.01	24	16.8	26578	PASS
442	198	50	100	67.7	158328	PASS
443	442	15	24	20.2	32010	PASS