
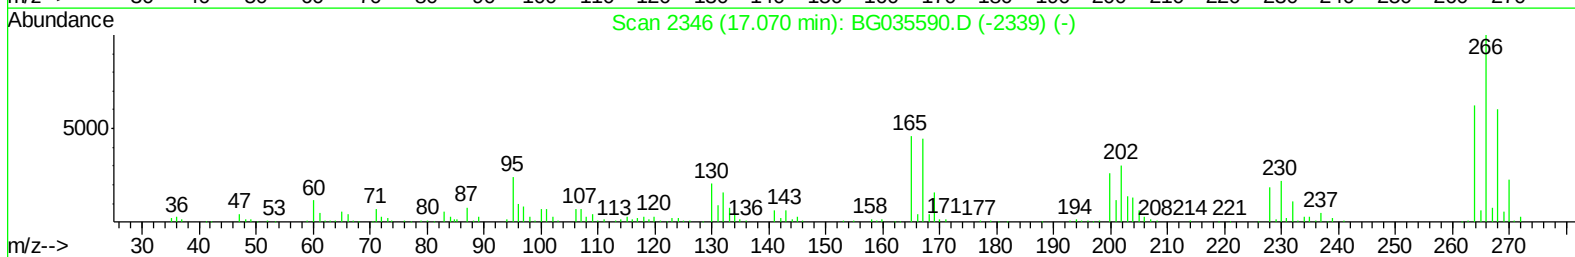
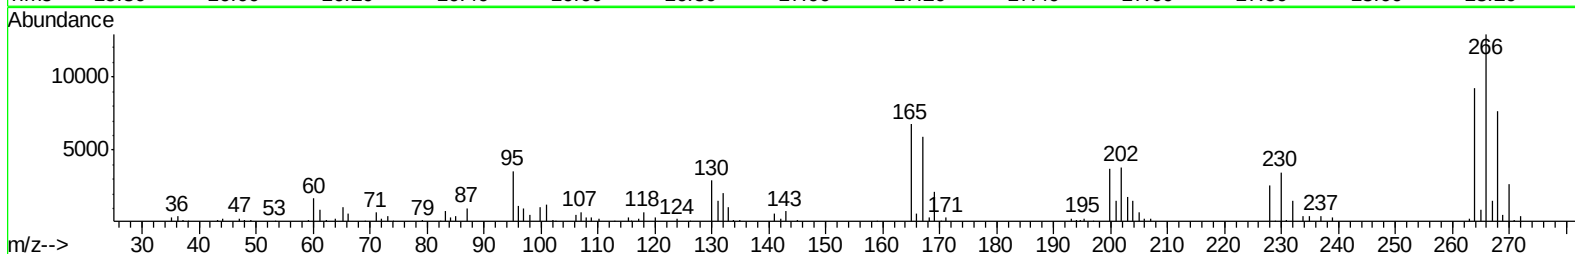


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071318\
Data File : BG035642.D
Acq On : 13 Jul 2018 23:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:44:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

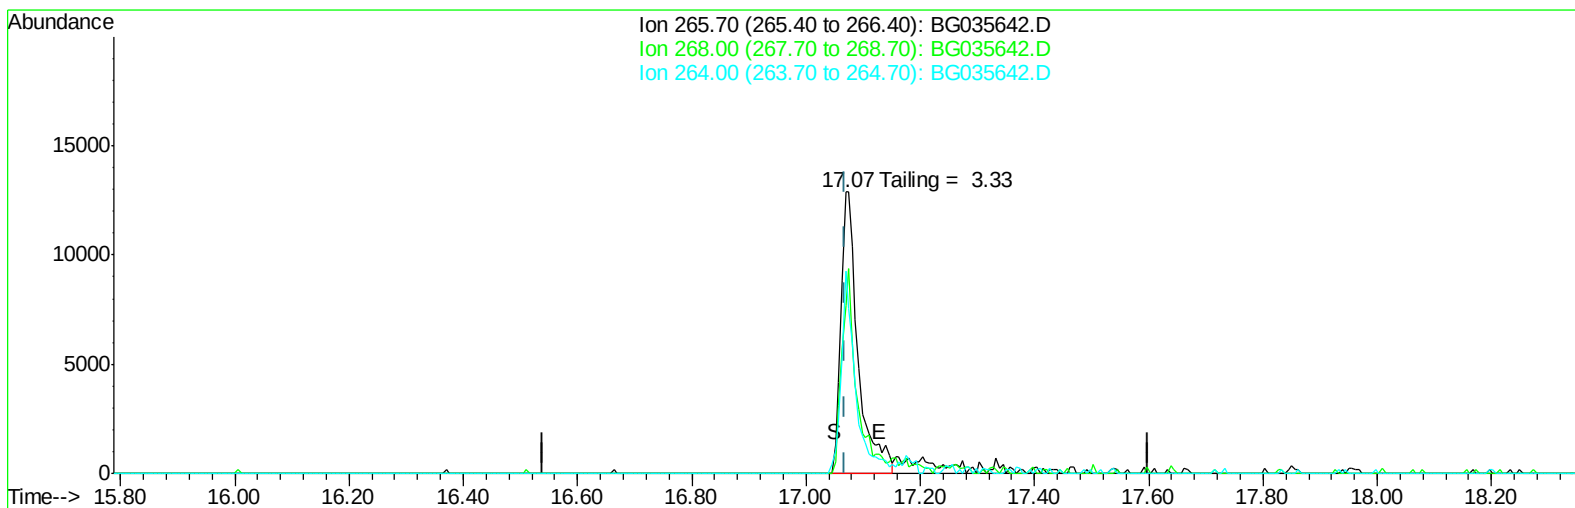

TIC: BG035642.D

(69) Pentachlorophenol (C)




17.069min (-0.001) 56394.60ng

response 27086

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.65
264.00	62.00	71.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071318\
Data File : BG035642.D
Acq On : 13 Jul 2018 23:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:44:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

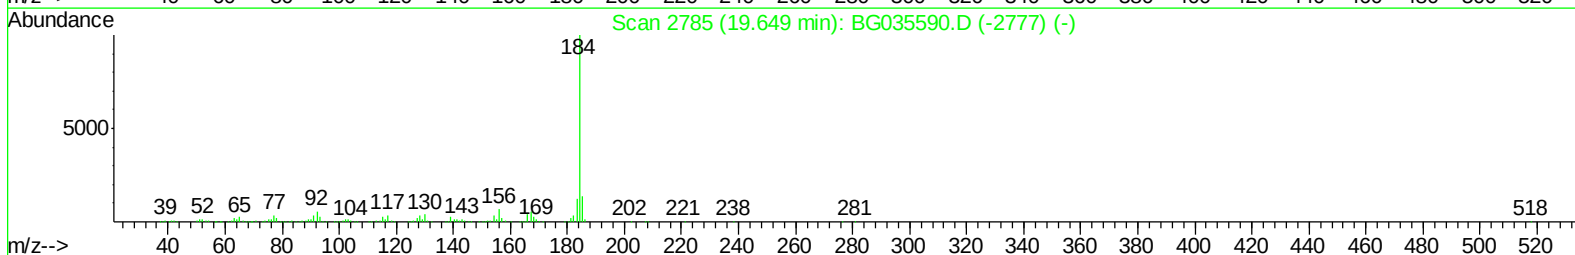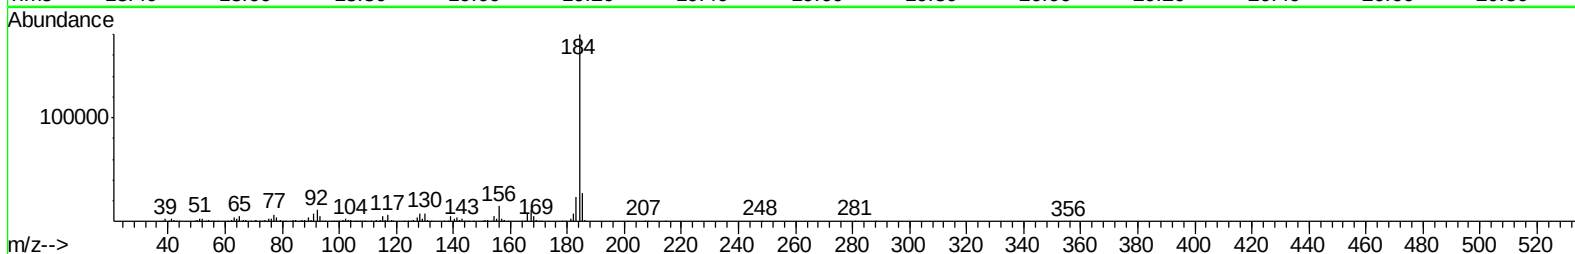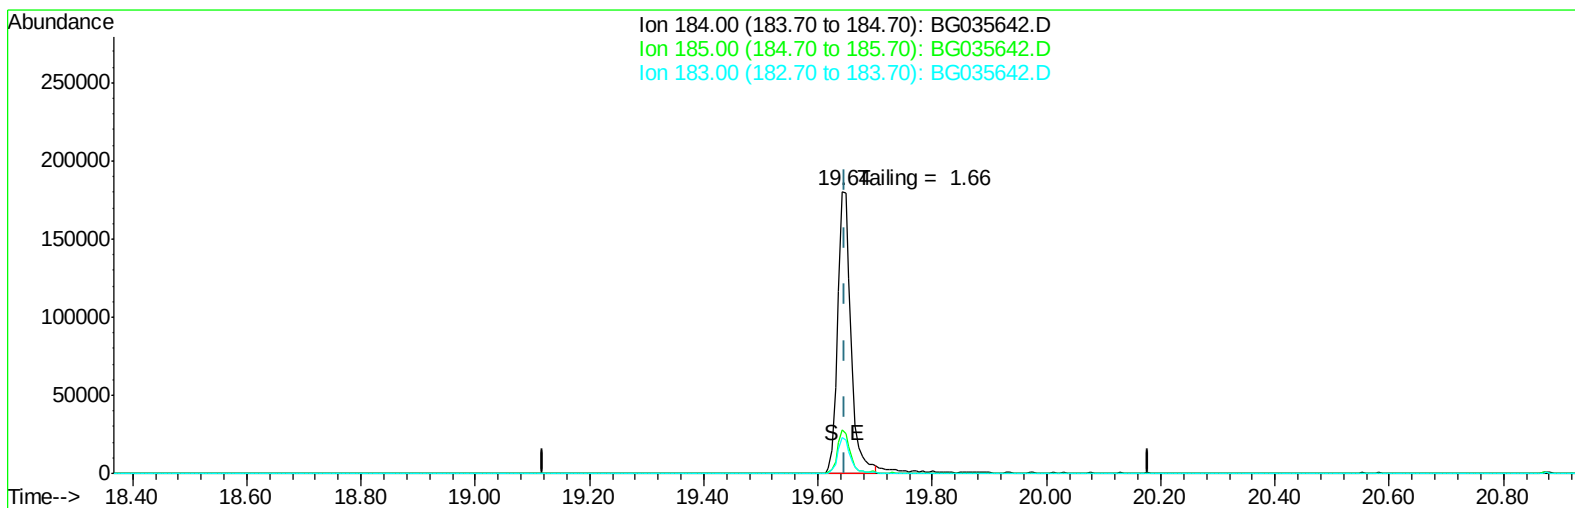

TIC: BG035642.D

(76) Benzidine

19.642min (-0.007) 198636.06ng

response 297665

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.38
183.00	13.30	12.81
0.00	0.00	0.00