
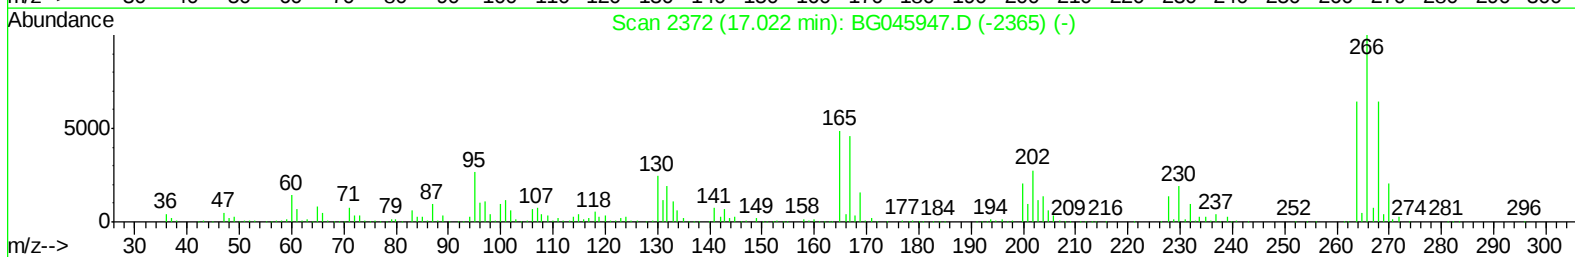
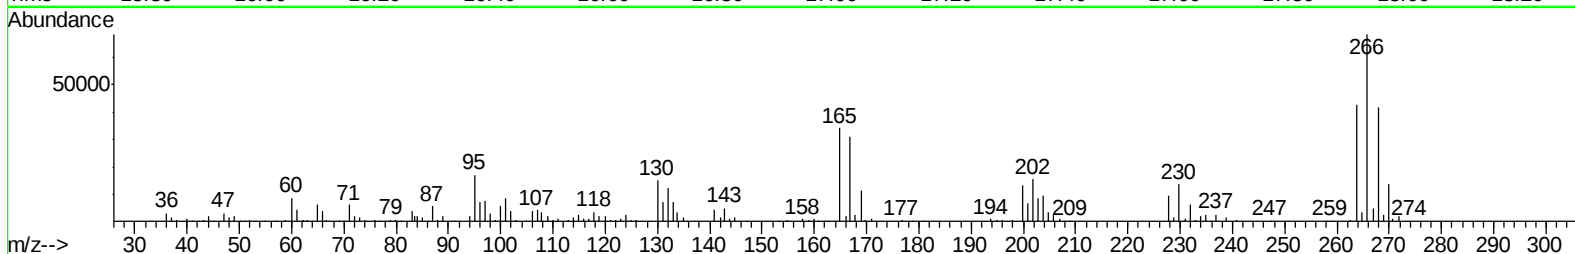


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071320\
Data File : BG046016.D
Acq On : 13 Jul 2020 8:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 01:52:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:58:53 2020
Response via : Initial Calibration

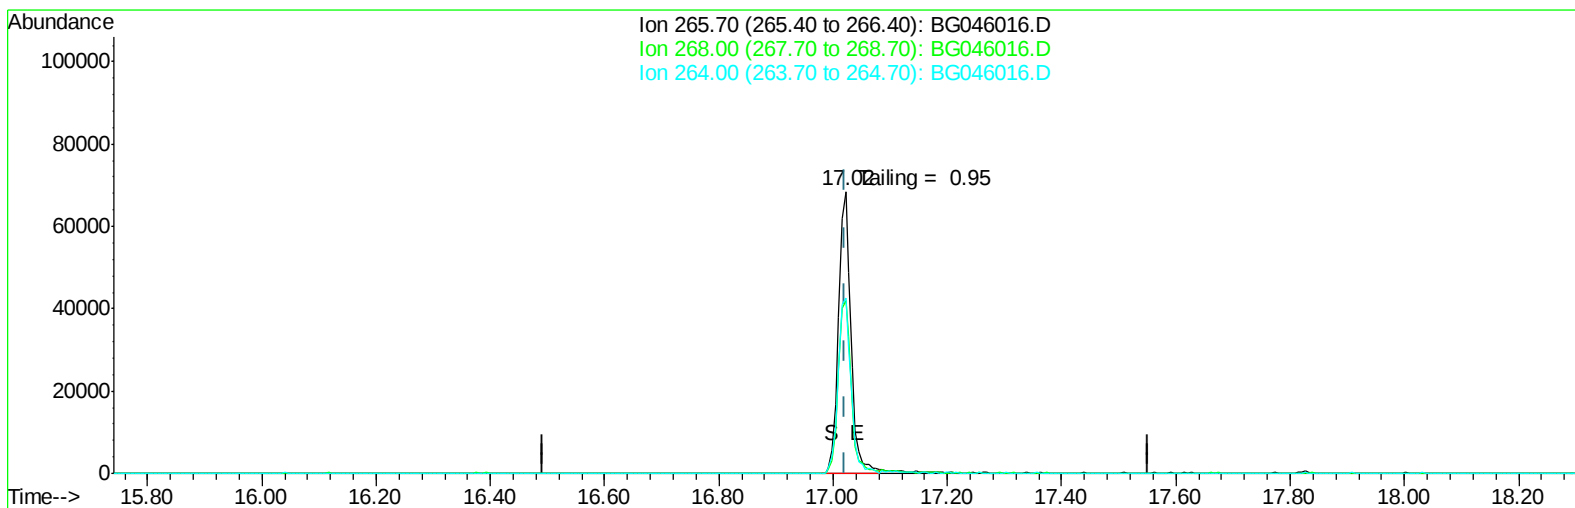

TIC: BG046016.D

(70) Pentachlorophenol (C)




17.021min (-0.001) 64935.72ng

response 105203

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	61.38
264.00	64.20	62.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071320\
 Data File : BG046016.D
 Acq On : 13 Jul 2020 8:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 01:52:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:58:53 2020
 Response via : Initial Calibration

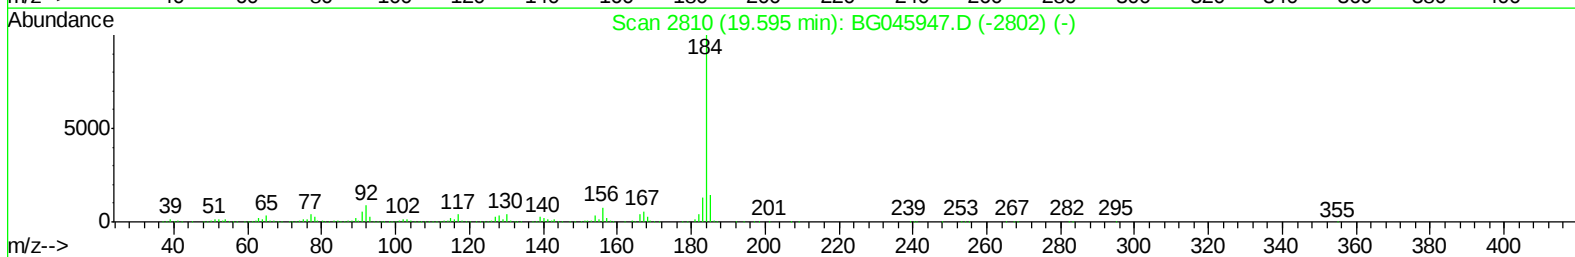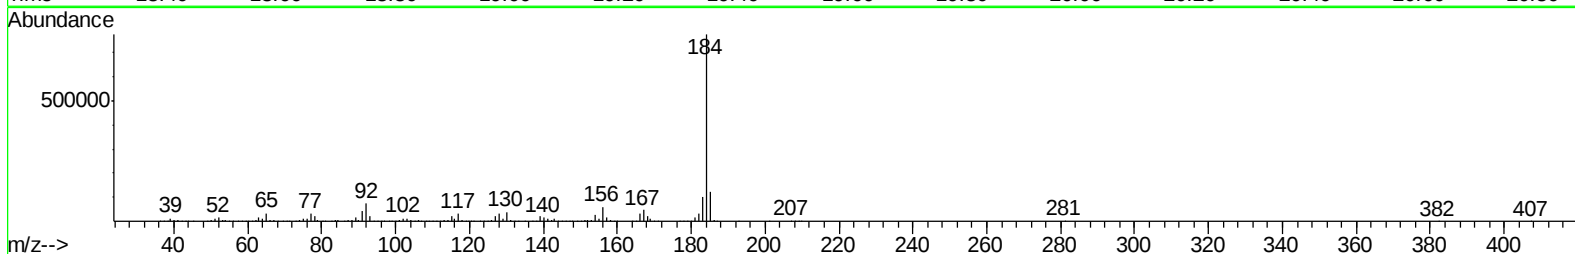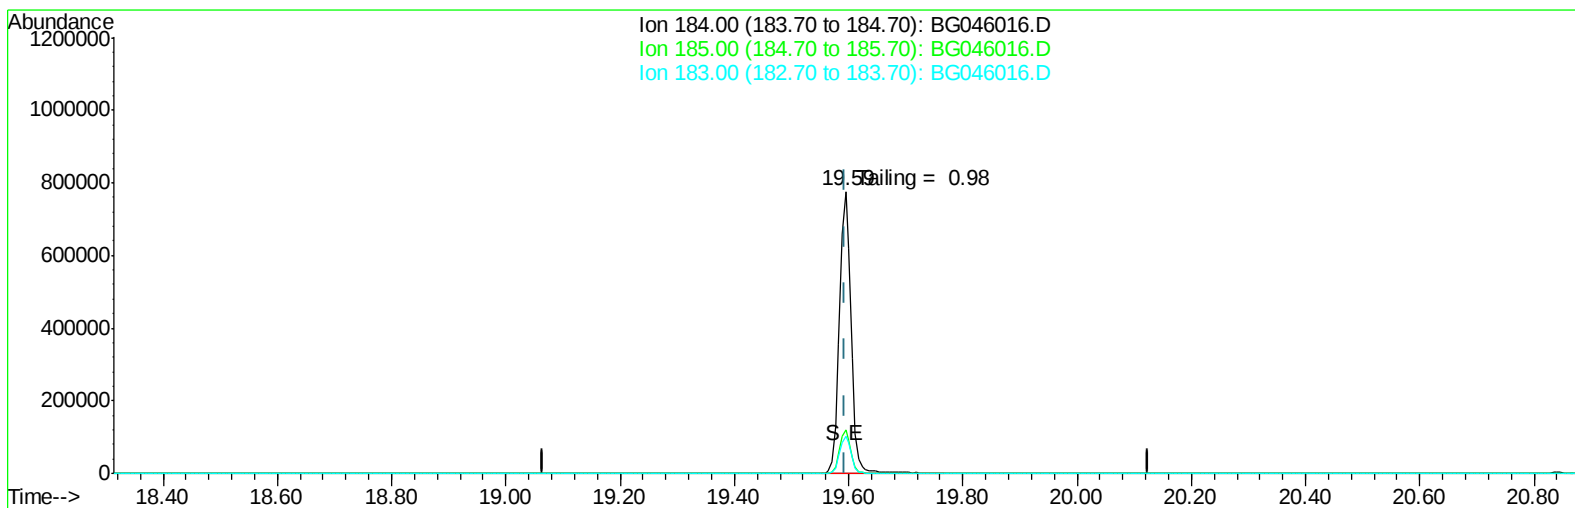

TIC: BG046016.D

(77) Benzidine

19.594min (-0.001) 184623.20ng

response 1108559

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	15.61
183.00	13.00	13.31
0.00	0.00	0.00