


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071320\
 Data File : BG046016.D
 Acq On : 13 Jul 2020 8:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:58:53 2020

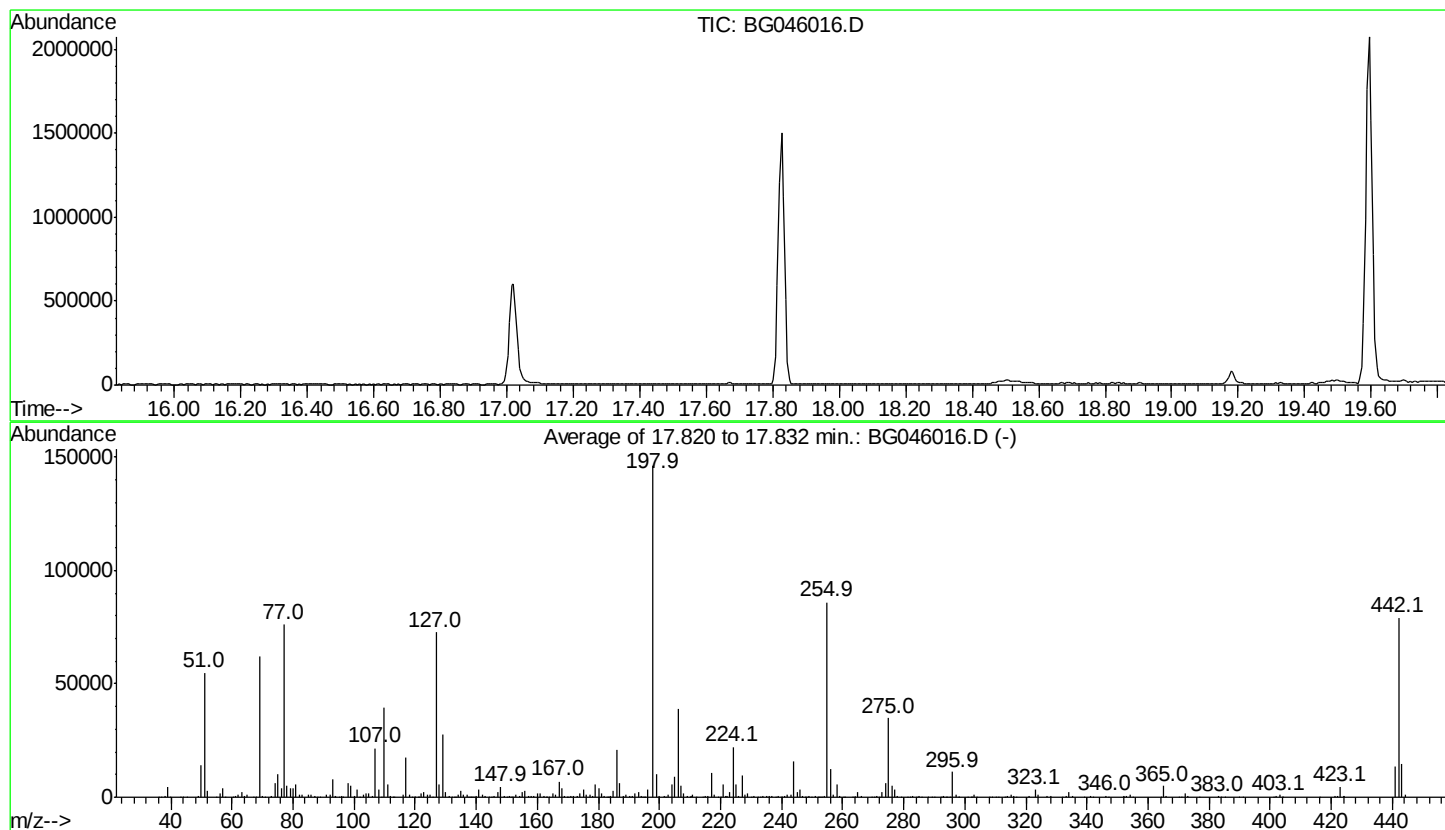

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	54896	PASS
68	69	0.00	2	0.4	230	PASS
69	198	0.00	100	42.6	62324	PASS
70	69	0.00	2	0.7	408	PASS
127	198	10	80	49.8	72810	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146285	PASS
199	198	5	9	7.1	10438	PASS
275	198	10	60	23.9	34994	PASS
365	198	1	100	3.4	5011	PASS
441	198	0.01	100	9.2	13457	PASS
442	198	50	100	54.1	79194	PASS
443	442	15	24	18.7	14827	PASS