
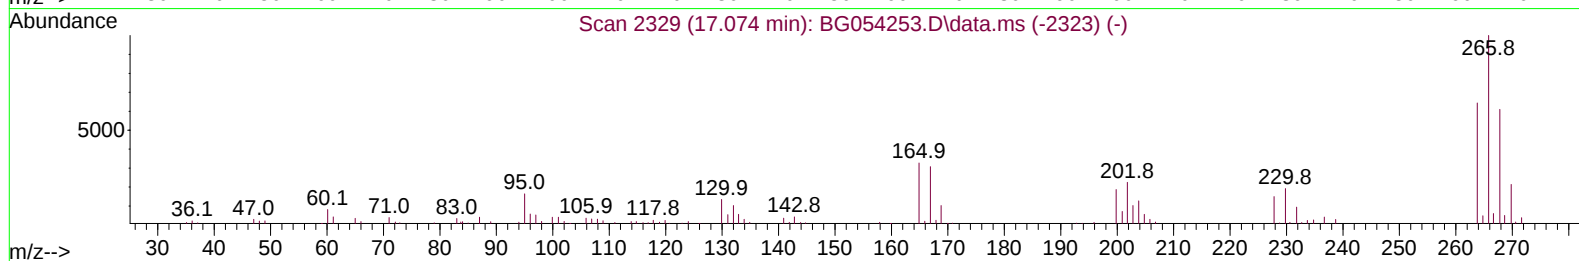
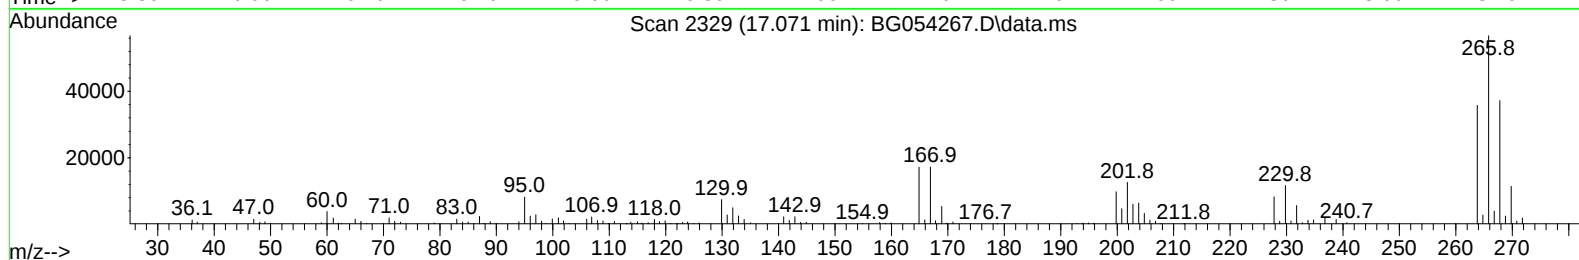


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054267.D
Acq On : 13 Jul 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:10:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

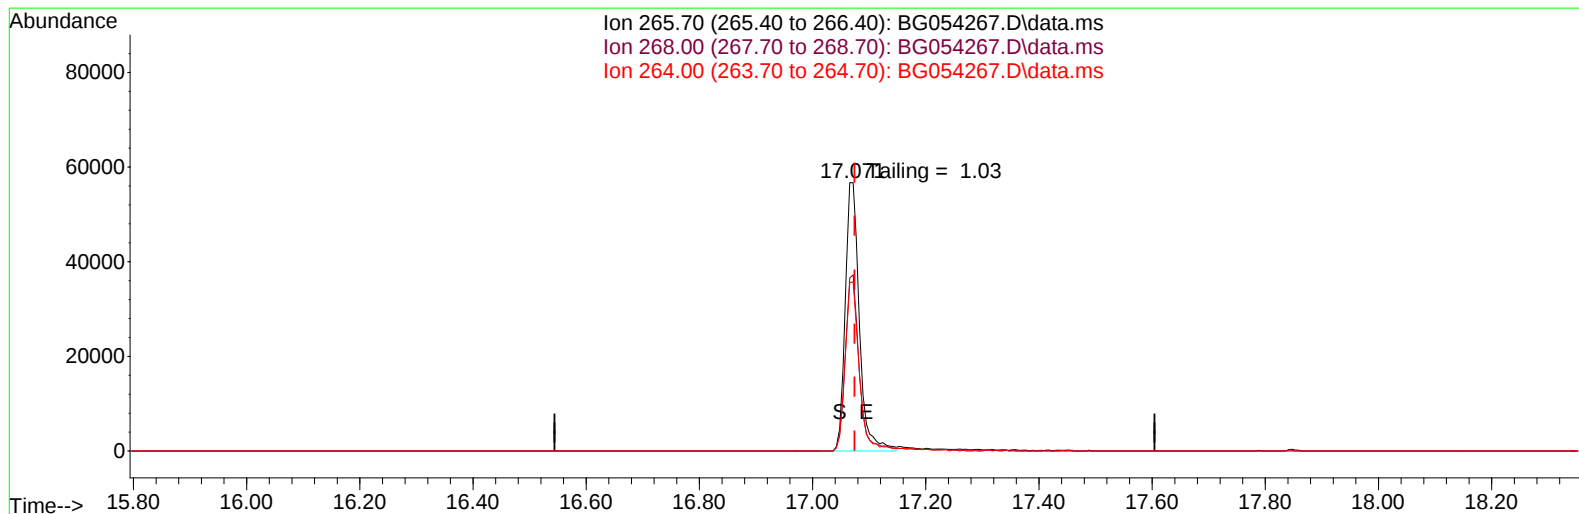

TIC: BG054267.D\data.ms

(70) Pentachlorophenol (C)




17.071min (-0.003) 29698.30 ng

response 100218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.64
264.00	66.20	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054267.D
Acq On : 13 Jul 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:10:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

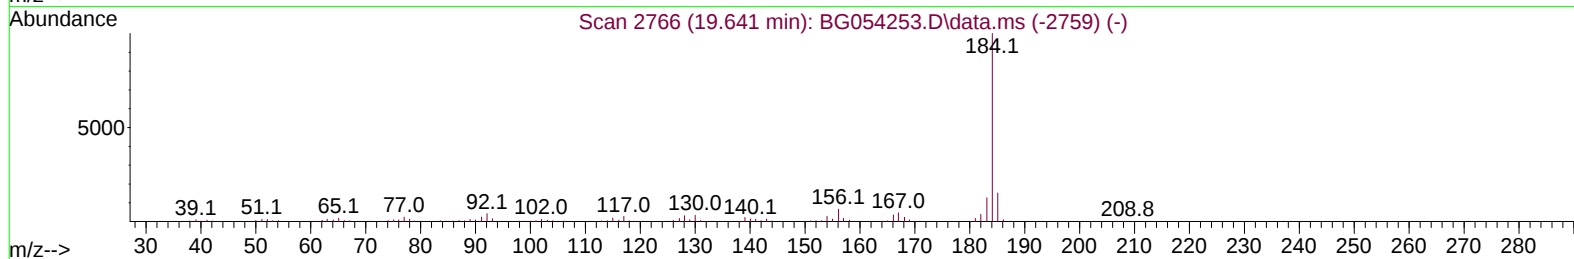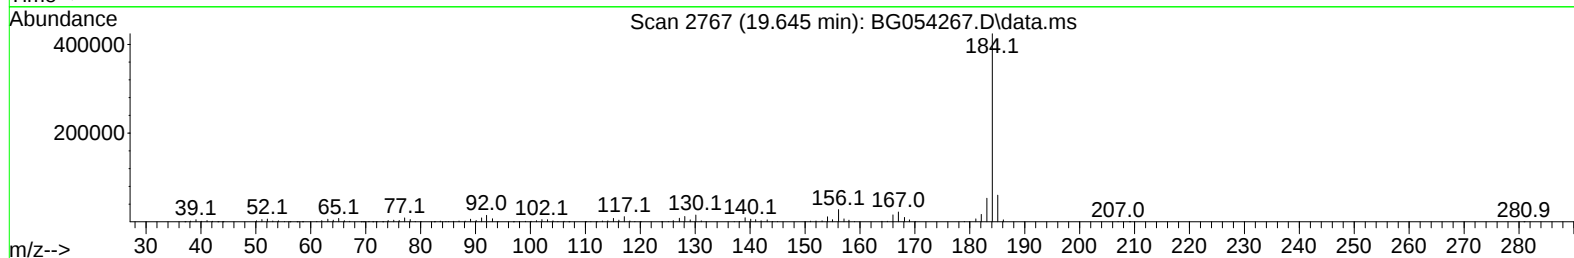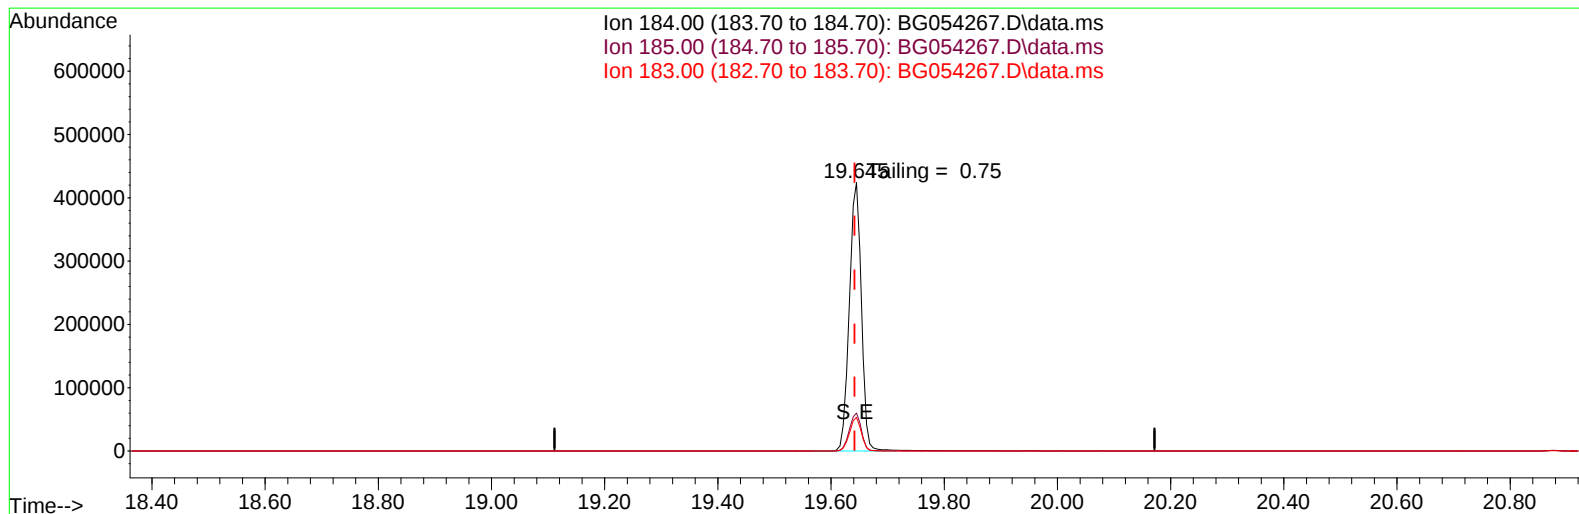

TIC: BG054267.D\data.ms

(77) Benzidine

19.645min (+ 0.004) 0.00 ng

response 630243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.15
183.00	11.10	12.51
0.00	0.00	0.00