

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
 Data File : BG054269.D
 Acq On : 13 Jul 2022 10:50
 Operator : CG/JU
 Sample : PB145921BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145921BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.614	372	379	391	rVB	221012	378574	17.53%	5.627%
2	7.206	642	650	665	rBV	230734	415966	19.26%	6.183%
3	8.040	785	792	801	rBB	56674	95916	4.44%	1.426%
4	9.204	983	990	999	rBV	149229	275331	12.75%	4.093%
5	10.849	1262	1270	1280	rBV	74140	137306	6.36%	2.041%
6	13.293	1679	1686	1695	rBV	527784	851986	39.45%	12.665%
7	14.668	1914	1920	1930	rBB	135773	224239	10.38%	3.333%
8	16.160	2167	2174	2187	rBV	515438	830141	38.44%	12.340%
9	17.412	2380	2387	2394	rBV	206698	333210	15.43%	4.953%
10	20.020	2825	2831	2838	rBV	1539044	2159692	100.00%	32.103%
11	21.683	3107	3114	3123	rBV2	294496	496928	23.01%	7.387%
12	24.926	3655	3666	3677	rVB	177470	499830	23.14%	7.430%
13	27.335	4065	4076	4083	rBV6	8092	28235	1.31%	0.420%




Sum of corrected areas: 6727354

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054269.D
Acq On : 13 Jul 2022 10:50
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

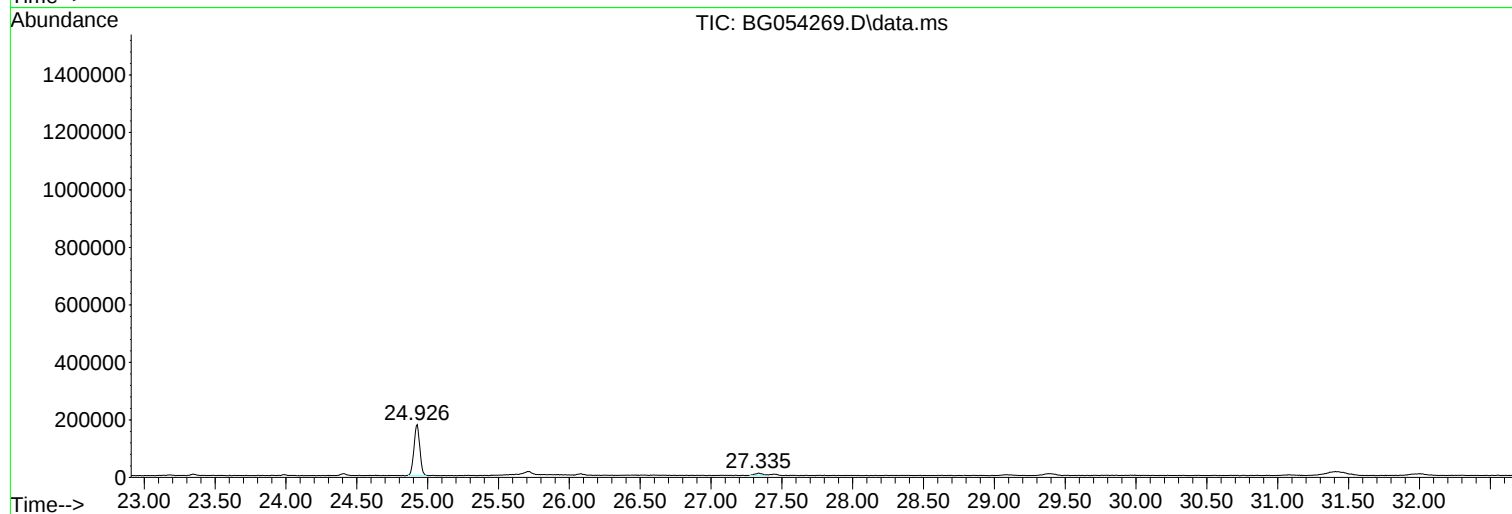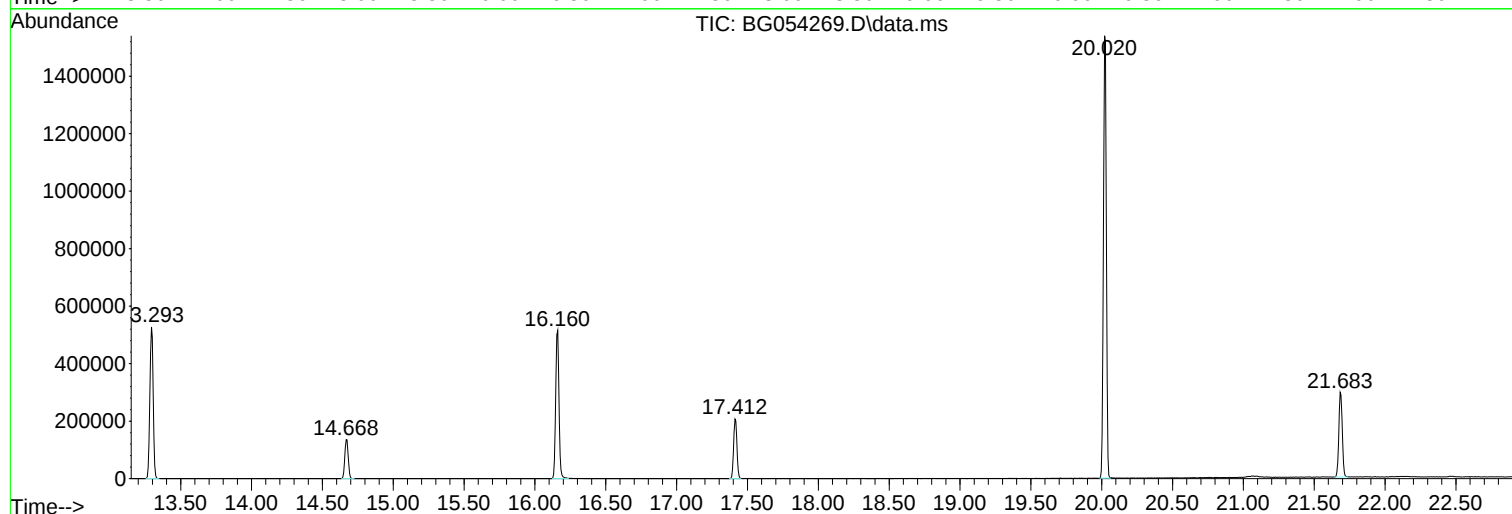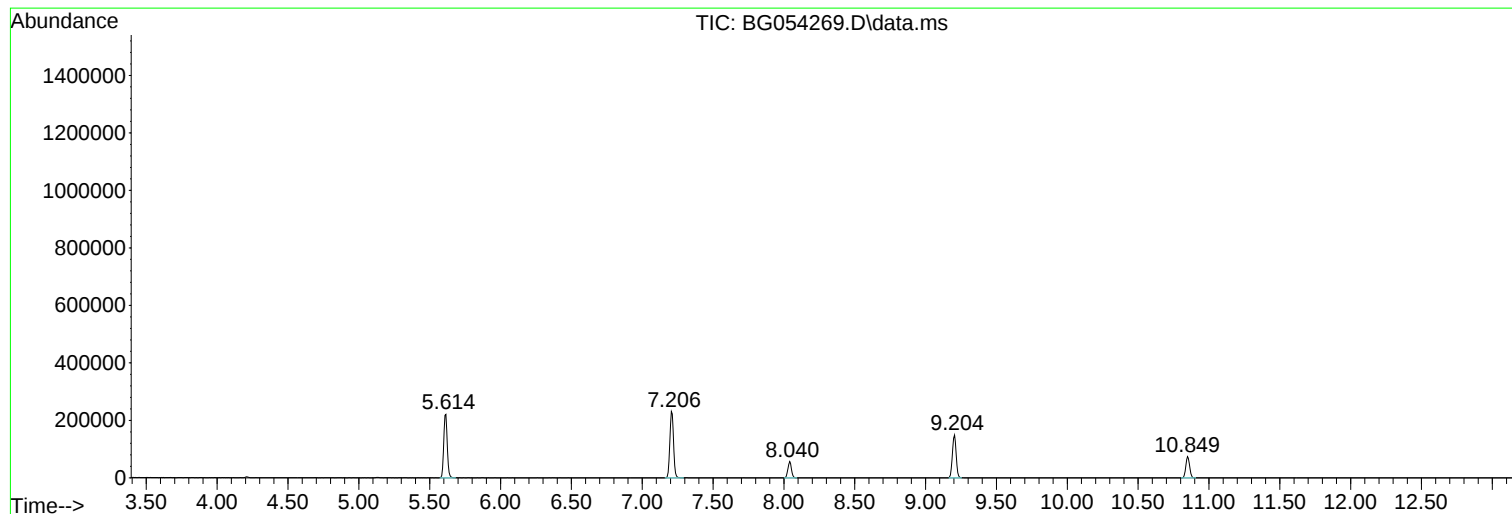

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054269.D
Acq On : 13 Jul 2022 10:50
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054269.D
Acq On : 13 Jul 2022 10:50
Operator : CG/JU
Sample : PB145921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------