


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
 Data File : BG054267.D
 Acq On : 13 Jul 2022 9:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 15:49:20 2022

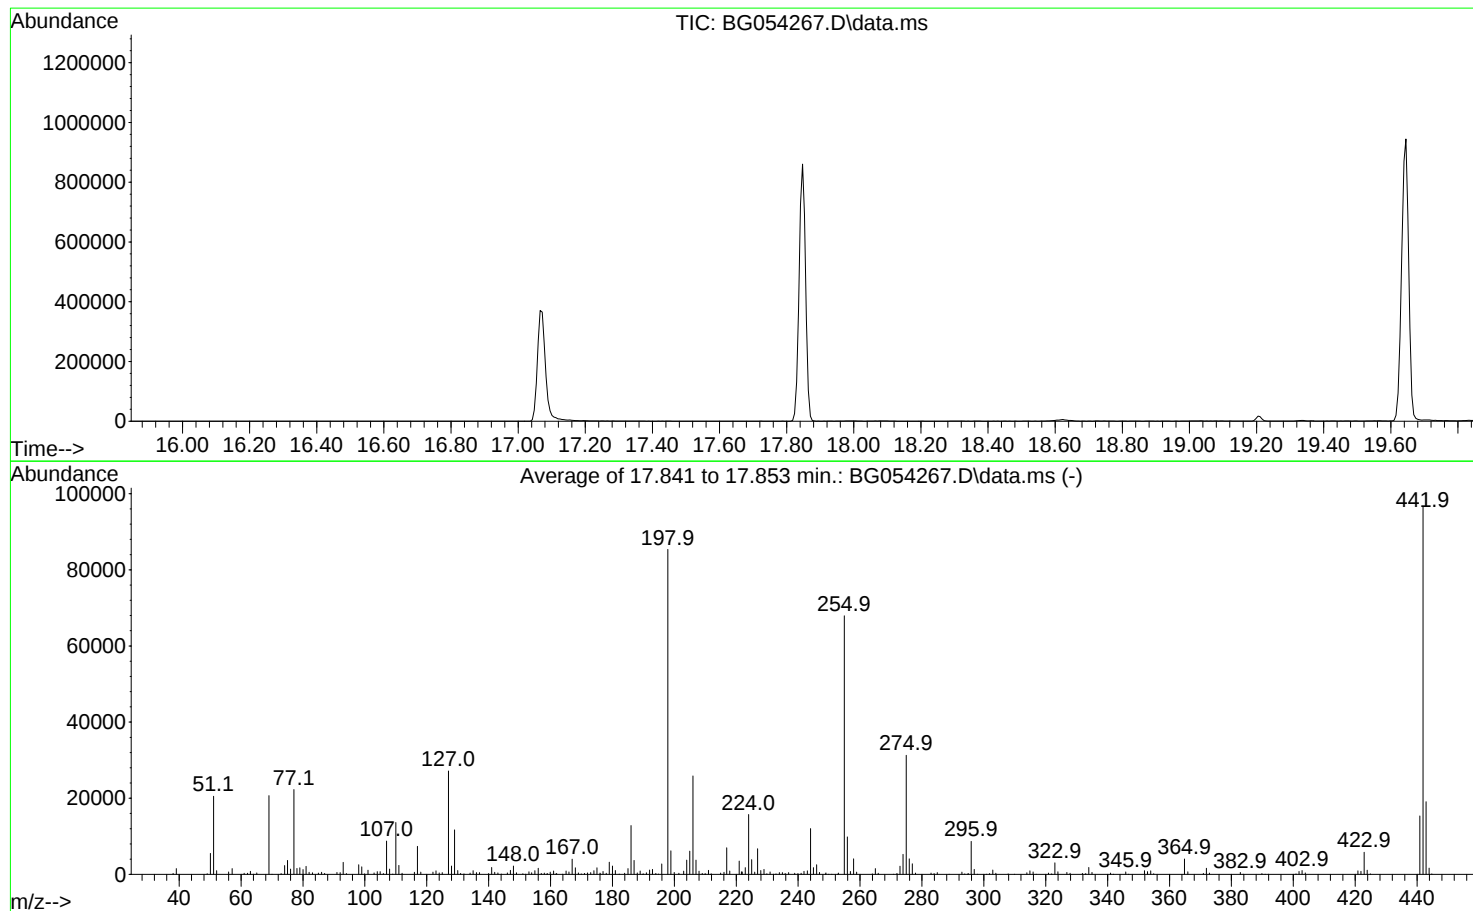

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	20516	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.2	20693	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	31.8	27157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85360	PASS
199	198	5	9	7.3	6199	PASS
275	198	10	60	36.7	31285	PASS
365	198	1	100	4.8	4059	PASS
441	198	0.01	100	18.0	15340	PASS
442	442	50	100	100.0	96635	PASS
443	442	15	24	19.8	19101	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/13/2022	BNA_G	<u>BG054267.D</u>
Compound Name	Response	Retention Time
DDT	383161	20.87
DDD	7615	20.43
DDE	0	19.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7615	390776	1.95

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054267.D
Acq On : 13 Jul 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 13 12:10:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

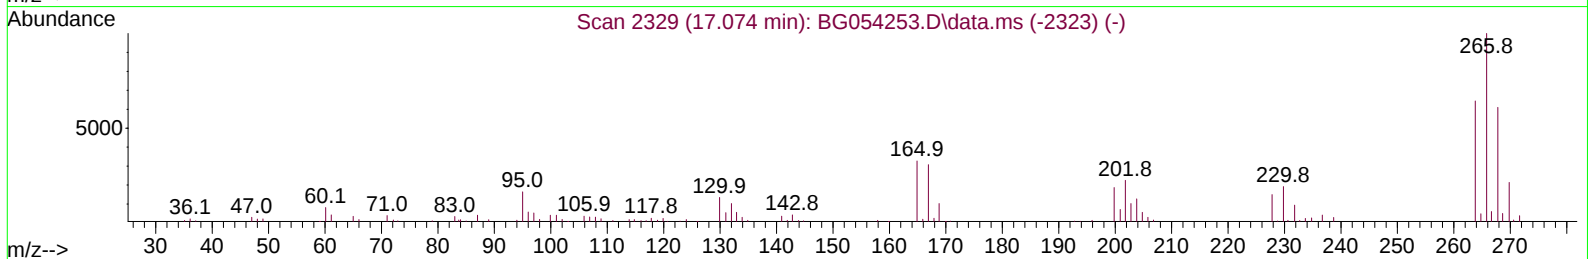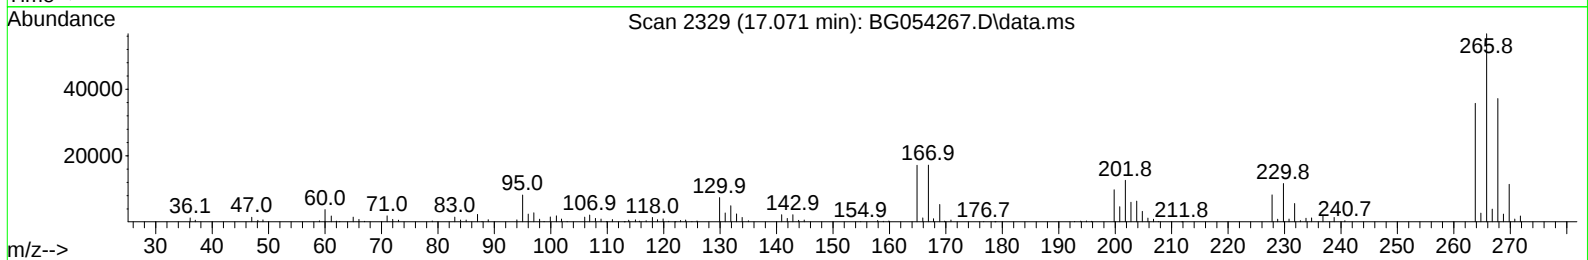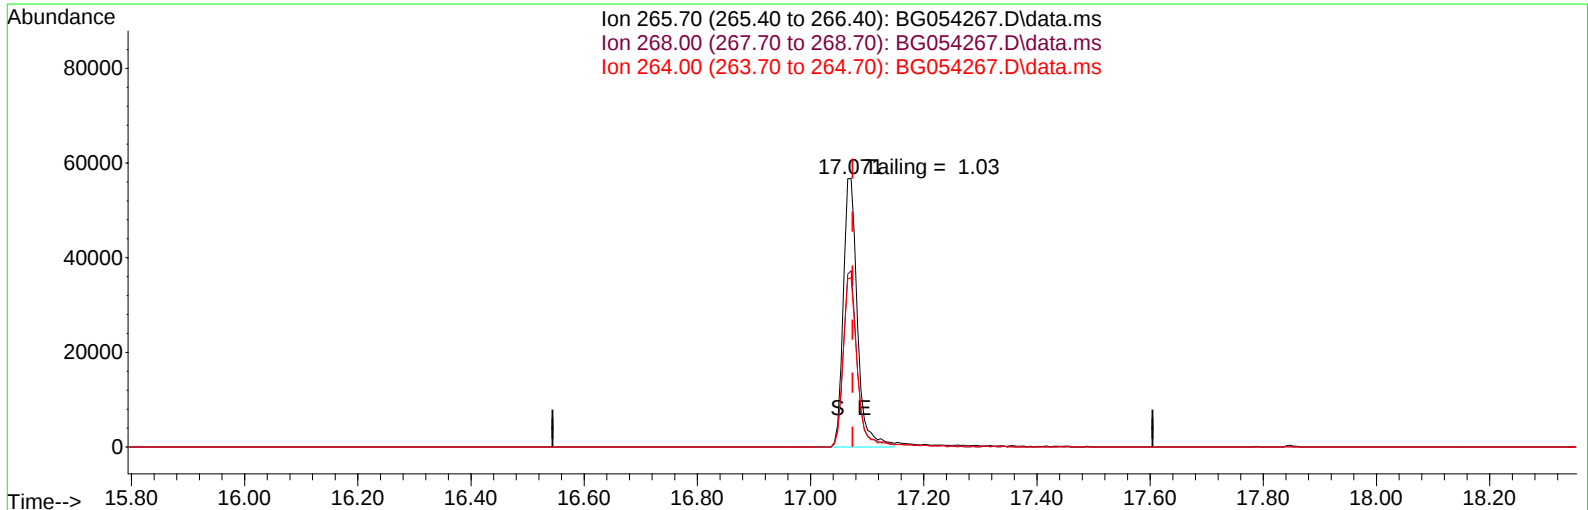

TIC: BG054267.D\data.ms

(70) Pentachlorophenol (C)

17.071min (-0.003) 29698.30 ng




response 100218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.64
264.00	66.20	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071322\
Data File : BG054267.D
Acq On : 13 Jul 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 13 12:10:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

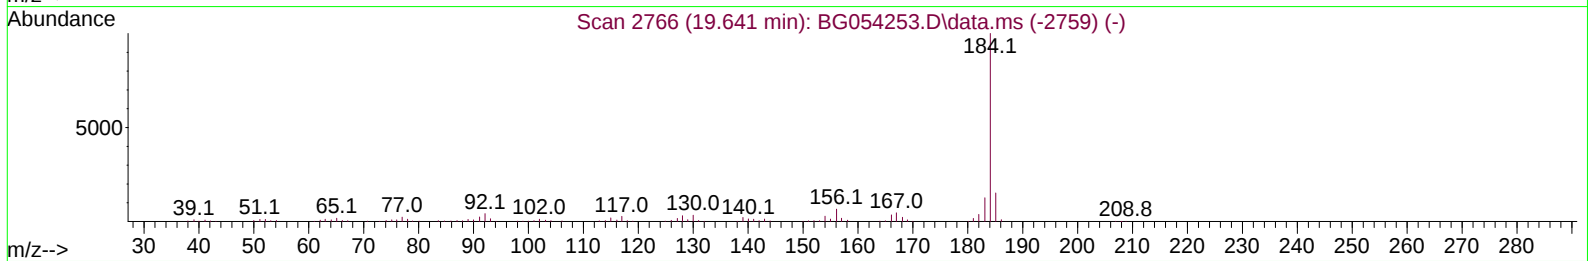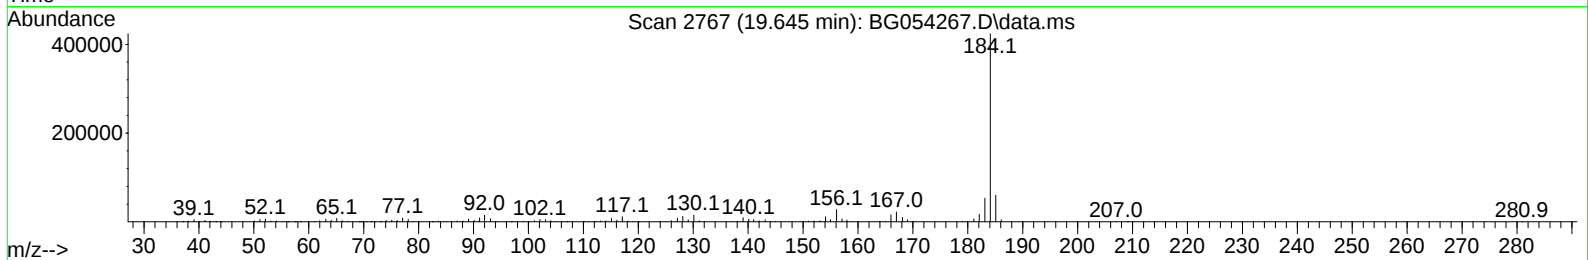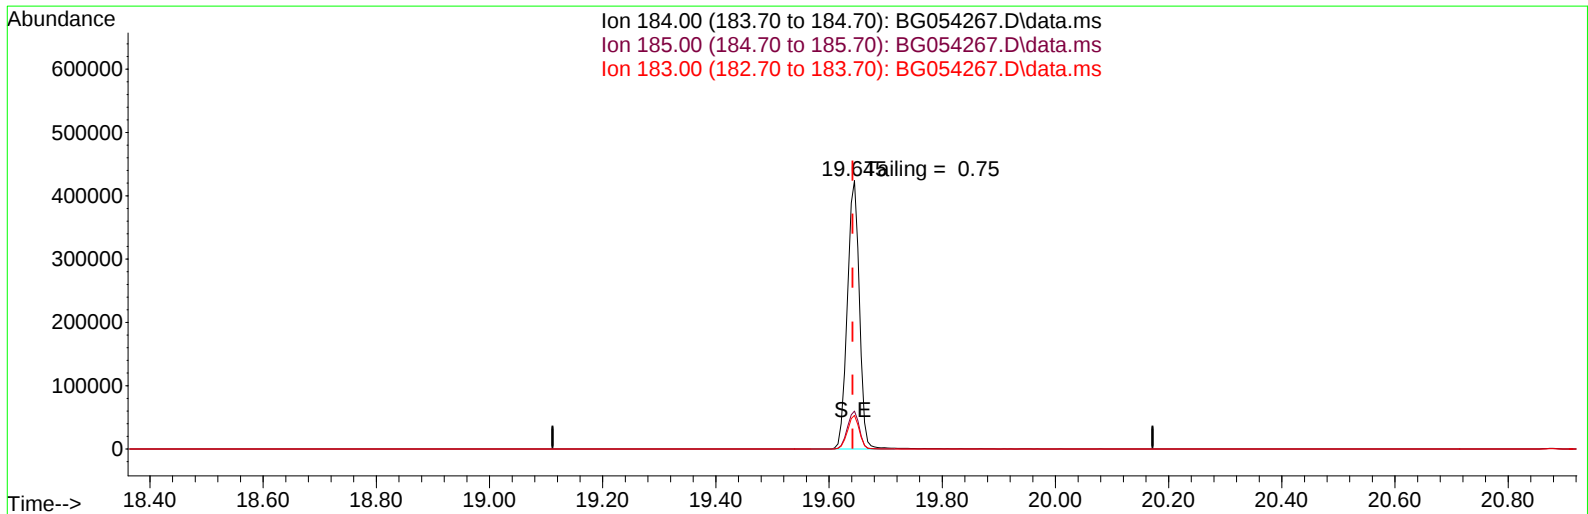

TIC: BG054267.D\data.ms

(77) Benzidine

19.645min (+ 0.004) 0.00 ng

response 630243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.15
183.00	11.10	12.51
0.00	0.00	0.00