
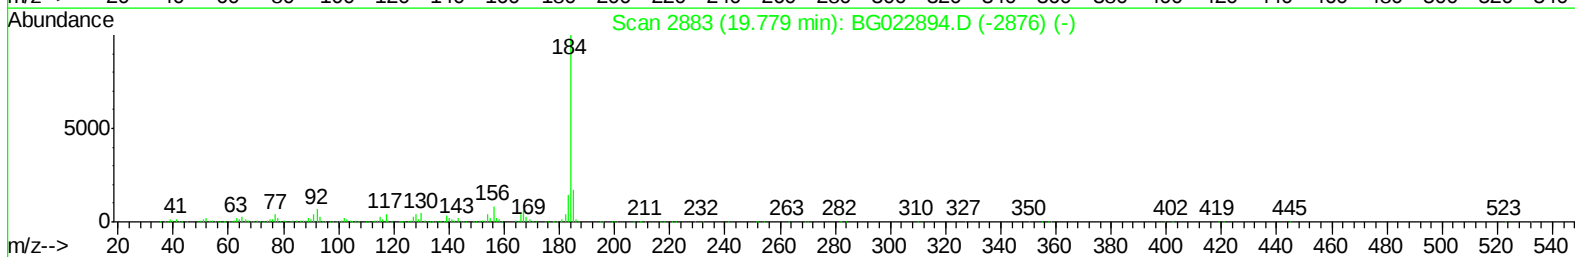
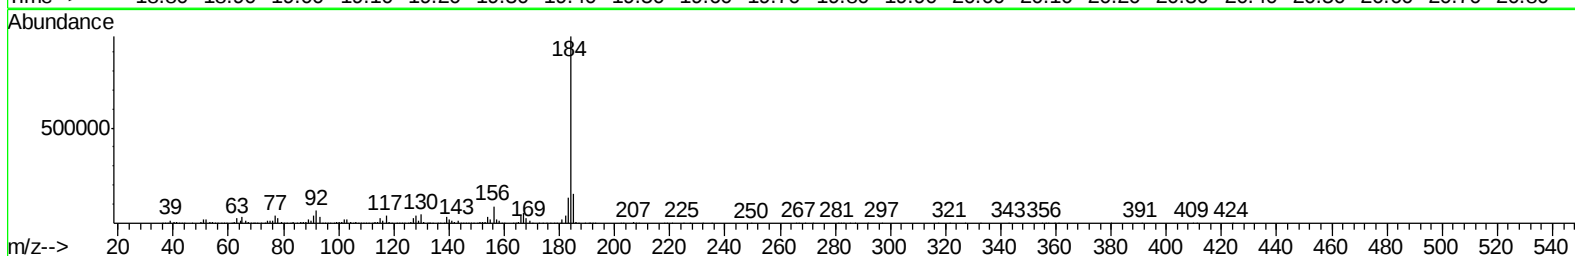


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071416\
Data File : BG023093.D
Acq On : 14 Jul 2016 9:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:56:45 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

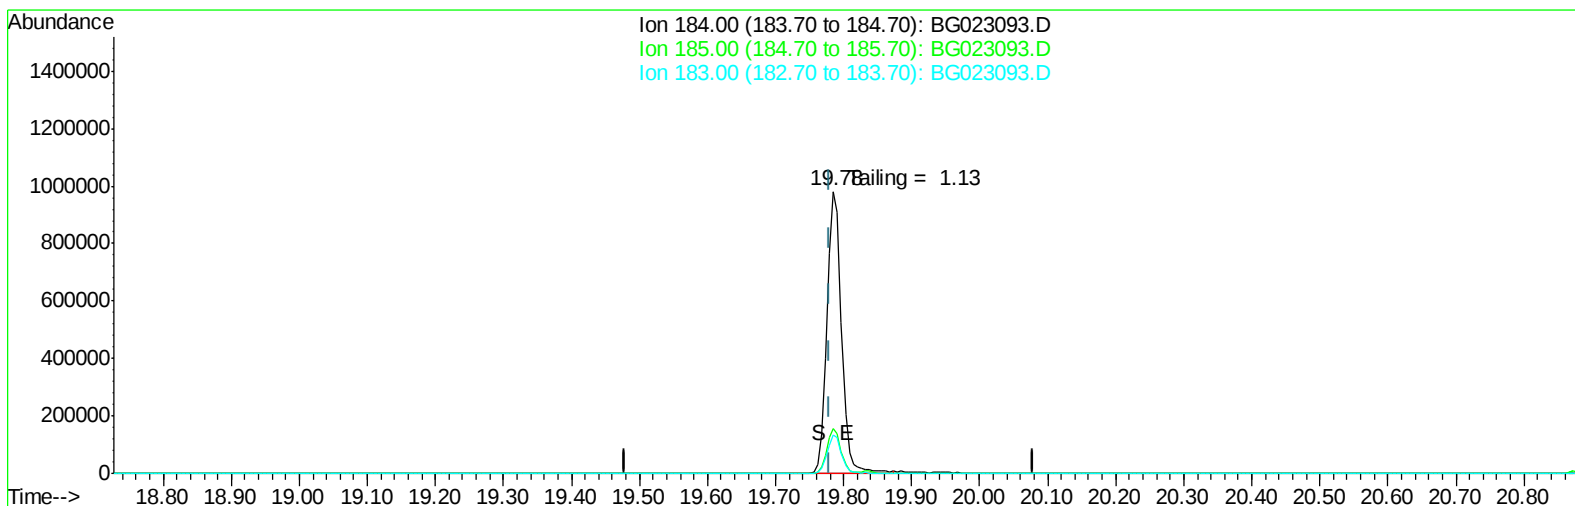

TIC: BG023093.D

(76) Benzidine




19.785min (+0.006) 8740.74ng

response 1476696

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.71
183.00	13.40	13.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071416\
Data File : BG023093.D
Acq On : 14 Jul 2016 9:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:56:45 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

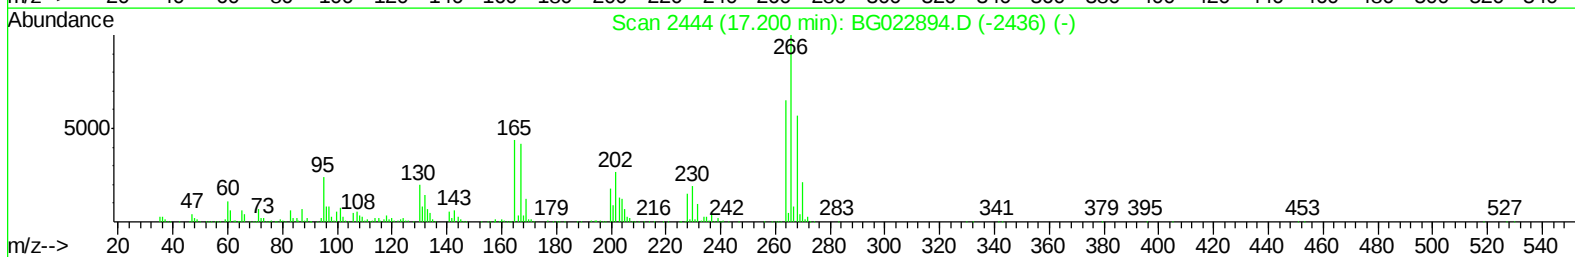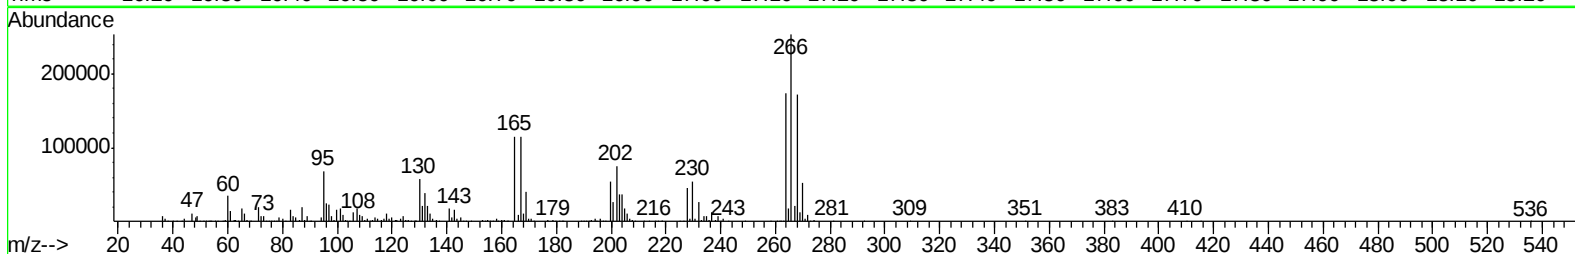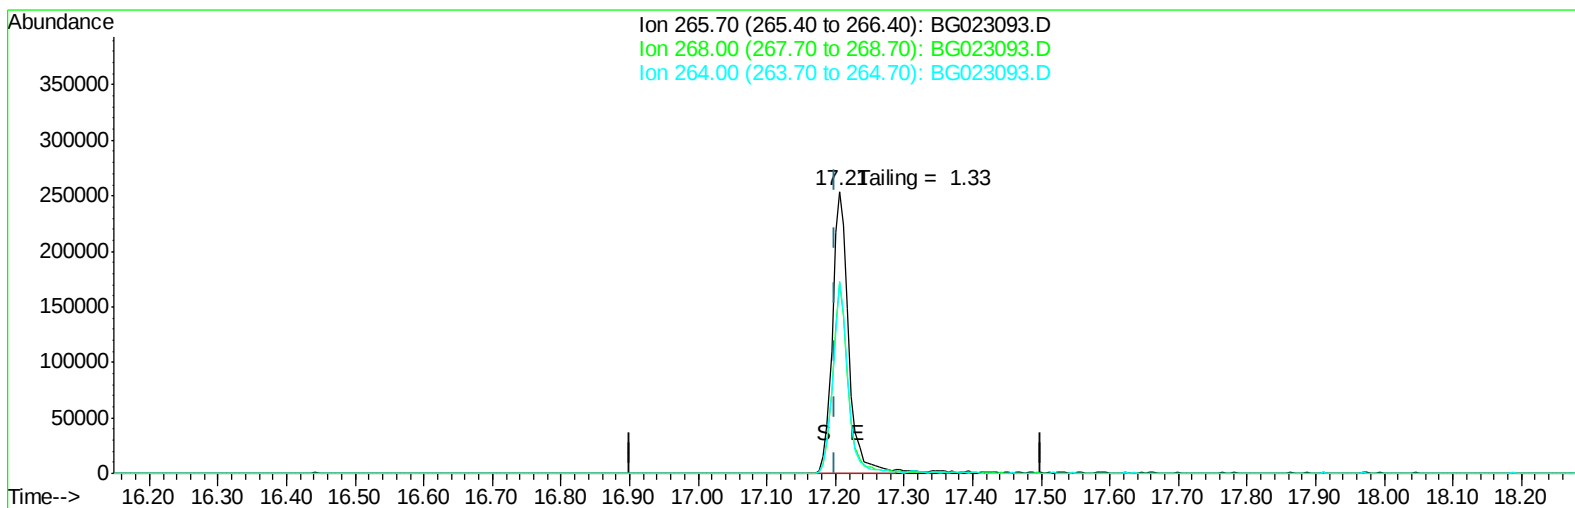

TIC: BG023093.D

(69) Pentachlorophenol (C)

17.206min (+0.006) 11359.29ng

response 420826

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.63
264.00	63.20	68.38
0.00	0.00	0.00