


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071416\
 Data File : BG023093.D
 Acq On : 14 Jul 2016 9:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

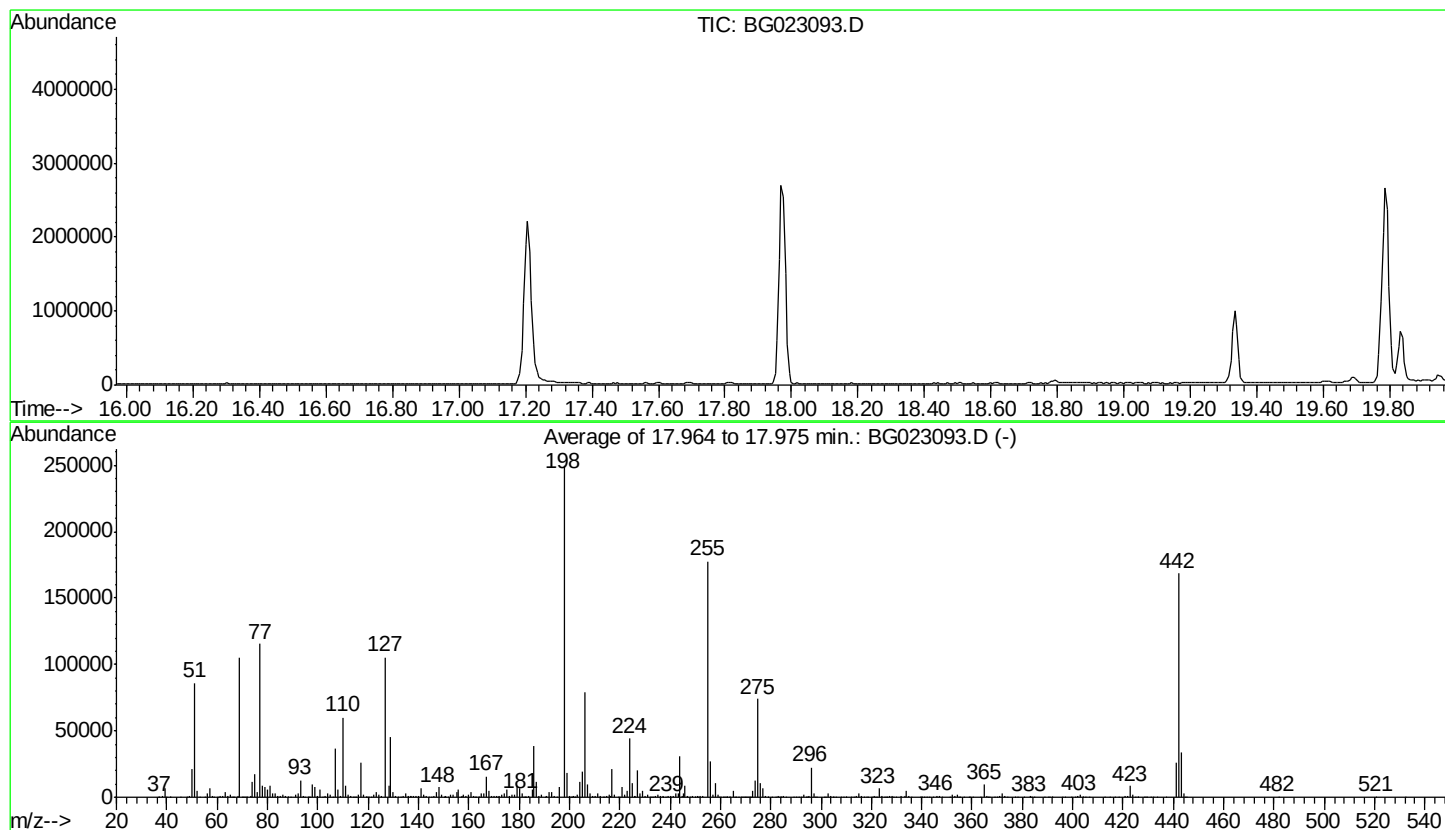

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	86125	PASS
68	69	0.00	2	0.6	665	PASS
69	198	0.00	100	42.0	104846	PASS
70	69	0.00	2	0.3	332	PASS
127	198	10	80	42.2	105360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	249664	PASS
199	198	5	9	7.2	17887	PASS
275	198	10	60	29.6	73890	PASS
365	198	1	100	3.8	9457	PASS
441	442	0.01	24	15.5	26102	PASS
442	198	50	100	67.5	168640	PASS
443	442	15	24	20.3	34180	PASS