
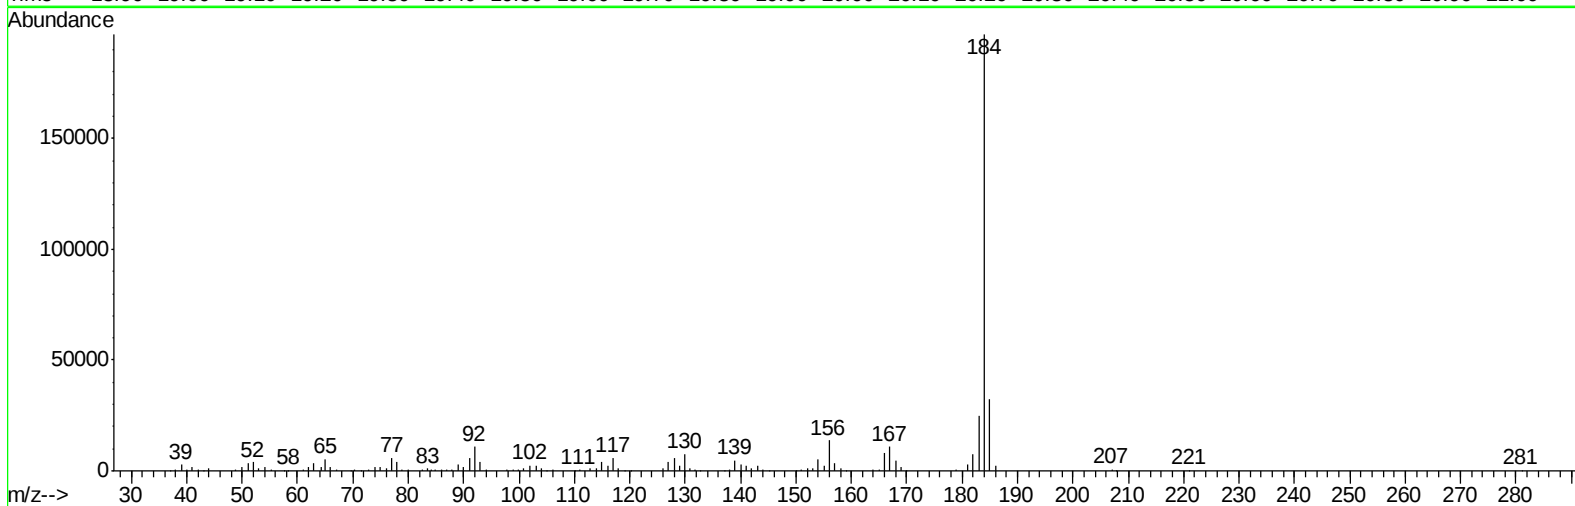


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071417\
Data File : BG027927.D
Acq On : 14 Jul 2017 16:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 03:38:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG071417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 16:10:34 2017
Response via : Initial Calibration

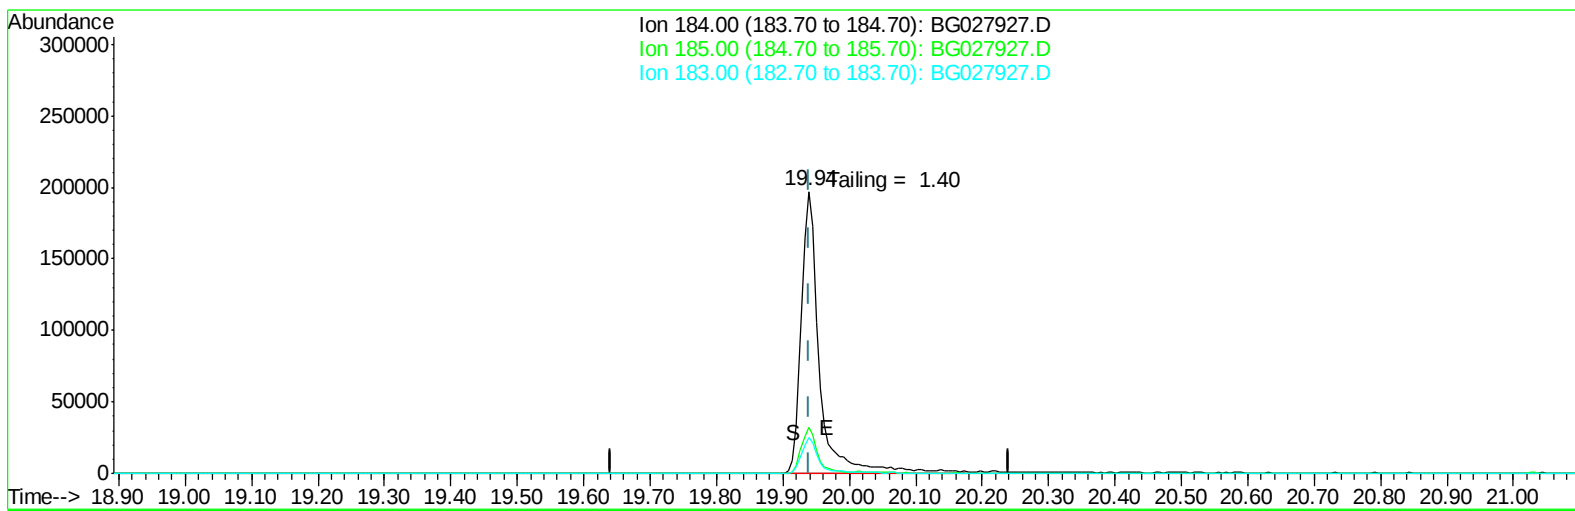

TIC: BG027927.D

(76) Benzidine



19.938min (-0.003) 0.00ng m

response 370676

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.53
183.00	13.80	12.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071417\
Data File : BG027927.D
Acq On : 14 Jul 2017 16:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 03:38:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG071417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 16:10:34 2017
Response via : Initial Calibration

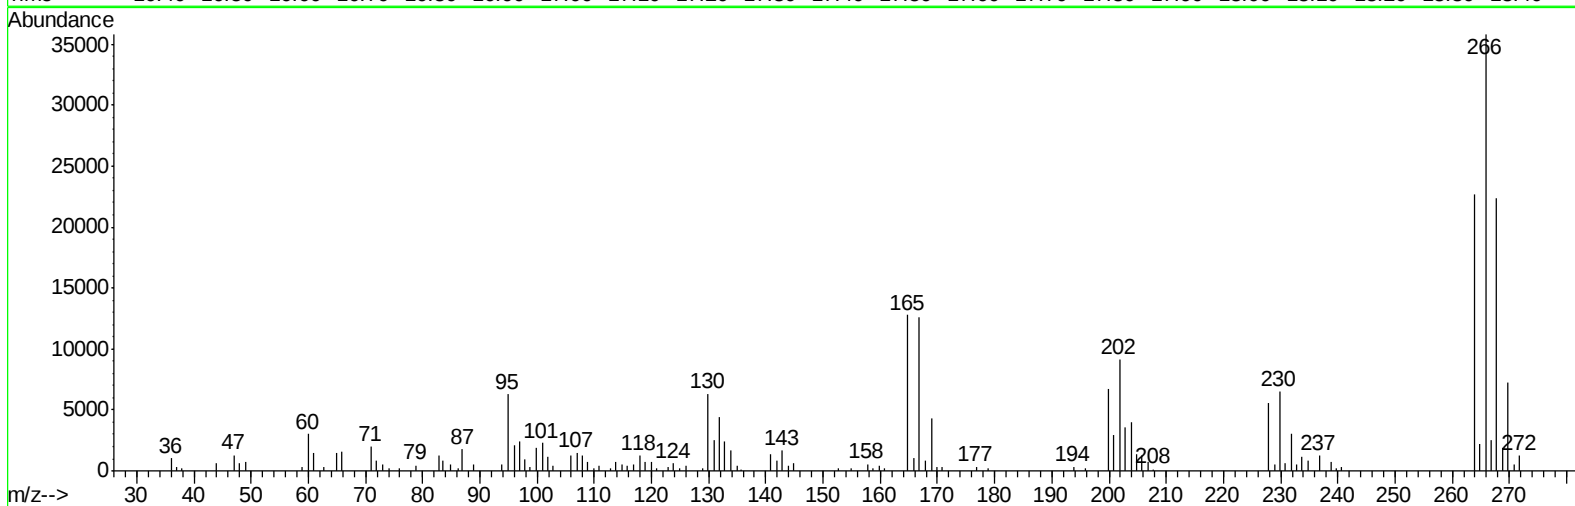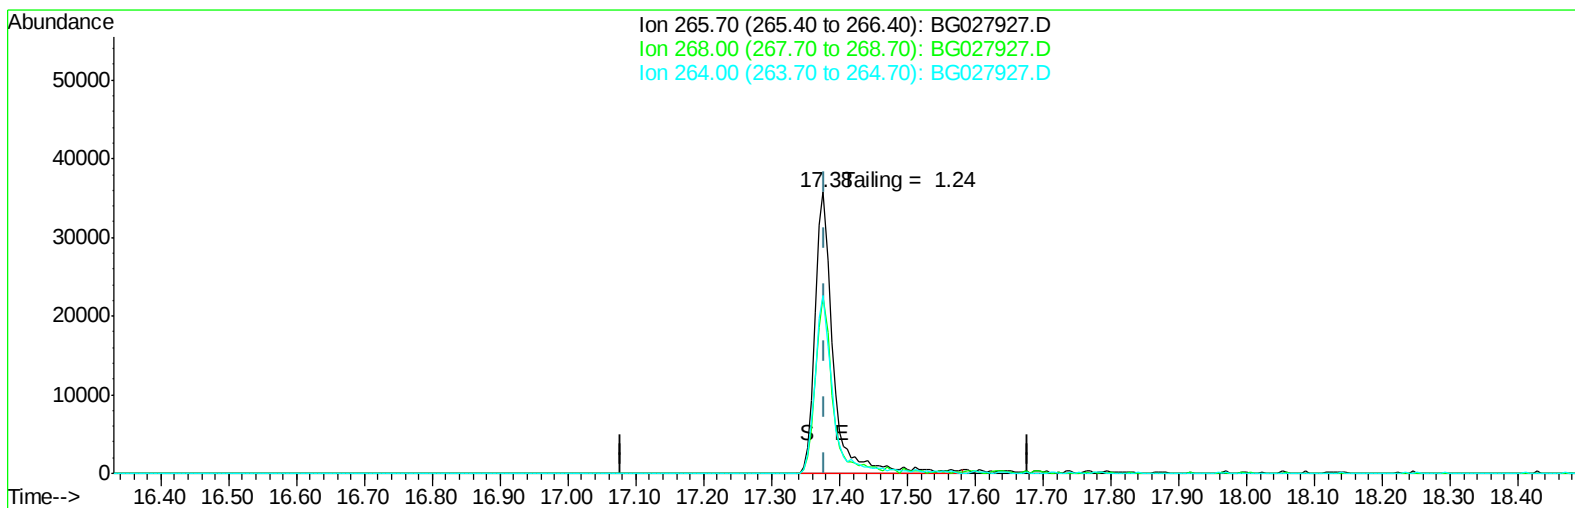

TIC: BG027927.D

(69) Pentachlorophenol (C)

17.376min (-0.003) 0.00ng

response 63918

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.53
264.00	62.60	63.37
0.00	0.00	0.00