


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071417\
 Data File : BG027918.D
 Acq On : 14 Jul 2017 10:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 14 16:10:34 2017

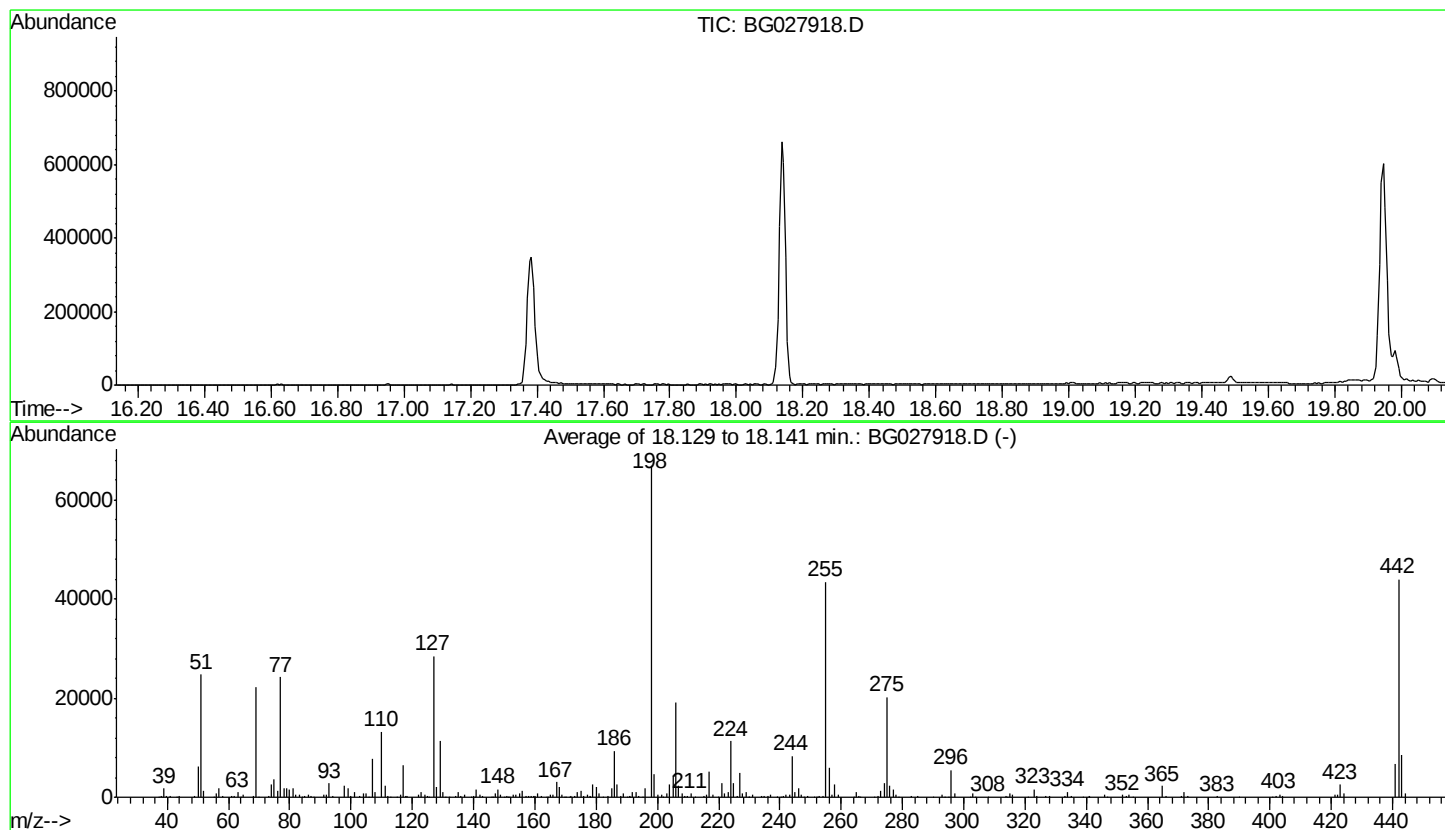

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	24741	PASS
68	69	0.00	2	1.7	388	PASS
69	198	0.00	100	33.3	22285	PASS
70	69	0.00	2	0.3	74	PASS
127	198	10	80	42.5	28400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66872	PASS
199	198	5	9	6.9	4583	PASS
275	198	10	60	30.2	20221	PASS
365	198	1	100	3.3	2220	PASS
441	442	0.01	24	15.2	6683	PASS
442	198	50	100	65.8	43984	PASS
443	442	15	24	19.4	8535	PASS