


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071417\
 Data File : BG027927.D
 Acq On : 14 Jul 2017 16:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 14 16:10:34 2017

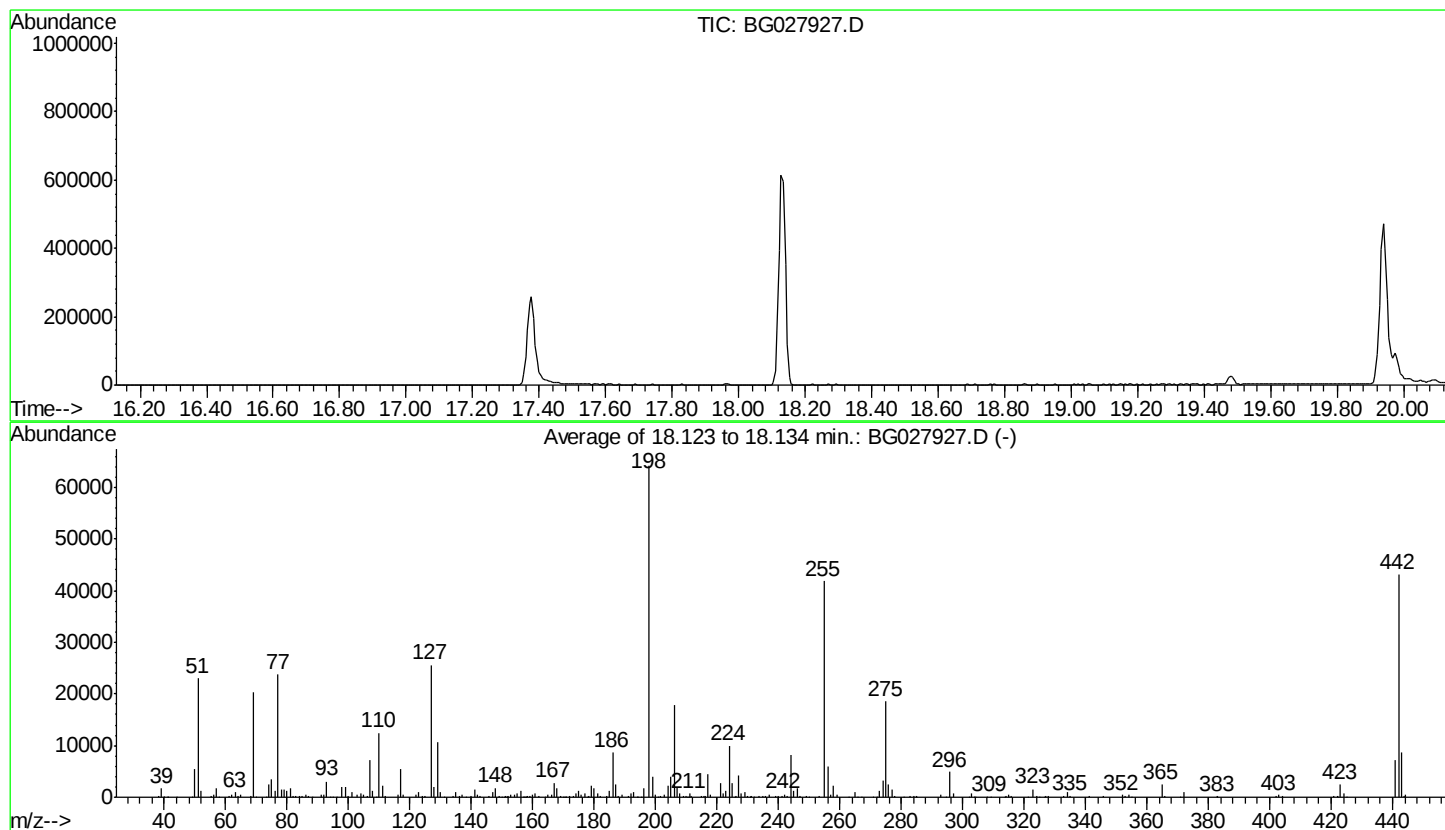

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	23005	PASS
68	69	0.00	2	1.8	369	PASS
69	198	0.00	100	31.9	20448	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	39.9	25616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64194	PASS
199	198	5	9	6.3	4016	PASS
275	198	10	60	28.8	18513	PASS
365	198	1	100	3.7	2379	PASS
441	442	0.01	24	16.6	7151	PASS
442	198	50	100	67.0	43026	PASS
443	442	15	24	20.3	8752	PASS