
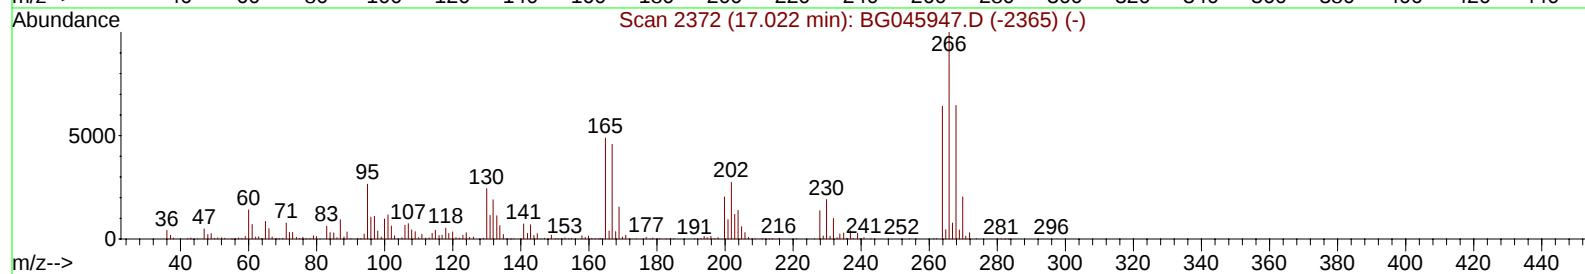
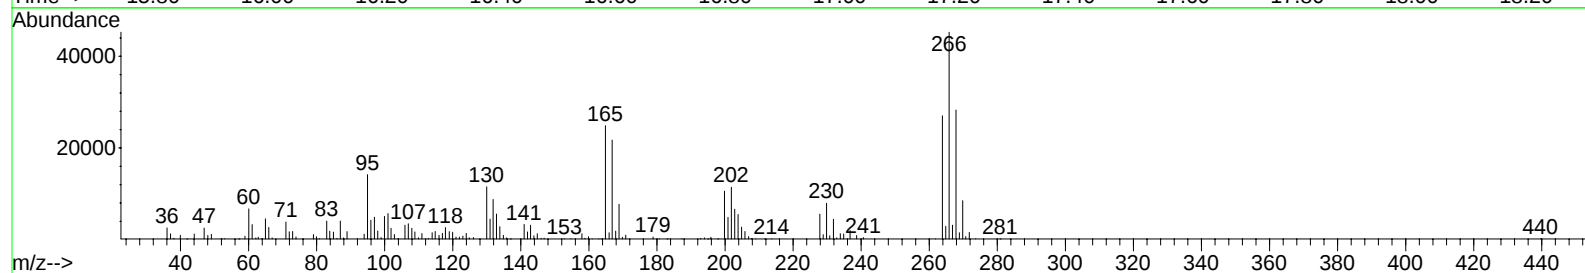


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071420\
 Data File : BG046029.D
 Acq On : 14 Jul 2020 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 16:29:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:58:53 2020
 Response via : Initial Calibration

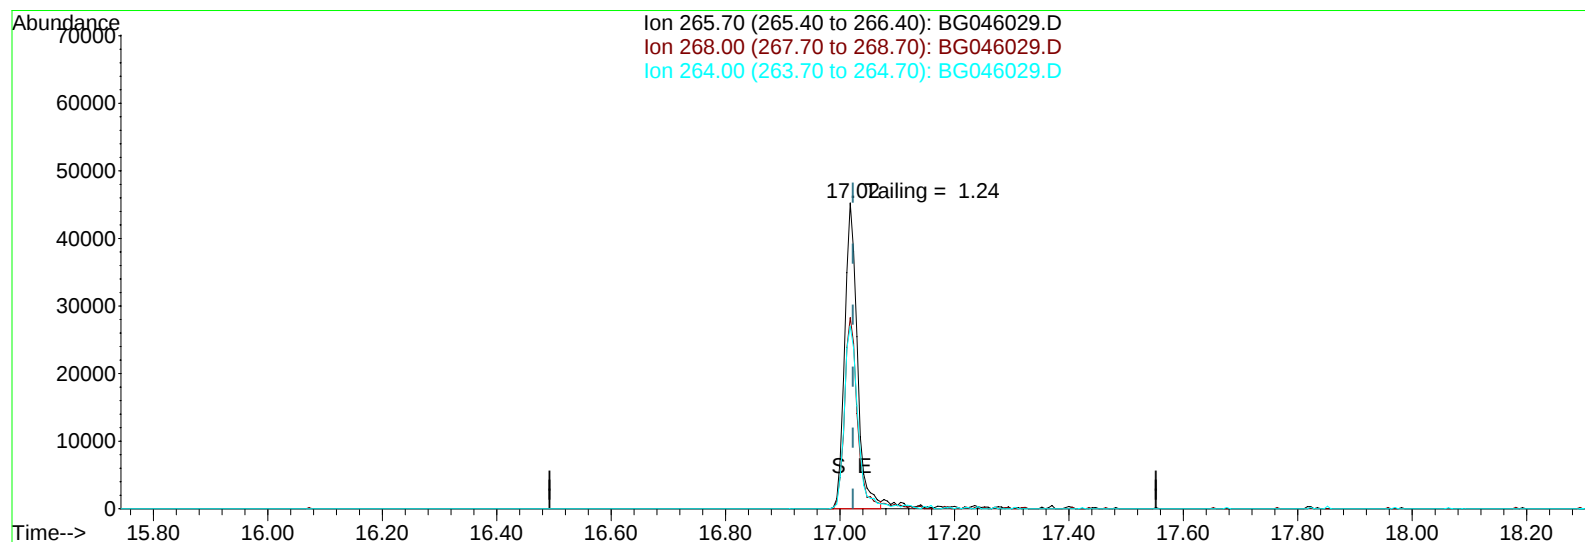

TIC: BG046029.D

(70) Pentachlorophenol (C)




17.018min (-0.004) 162354.46ng

response 68793

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	62.50
264.00	64.20	59.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071420\
 Data File : BG046029.D
 Acq On : 14 Jul 2020 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 16:29:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:58:53 2020
 Response via : Initial Calibration

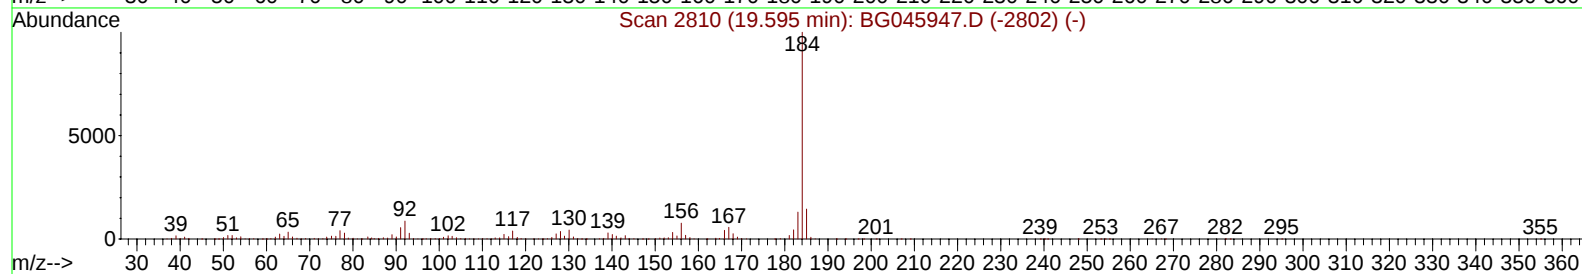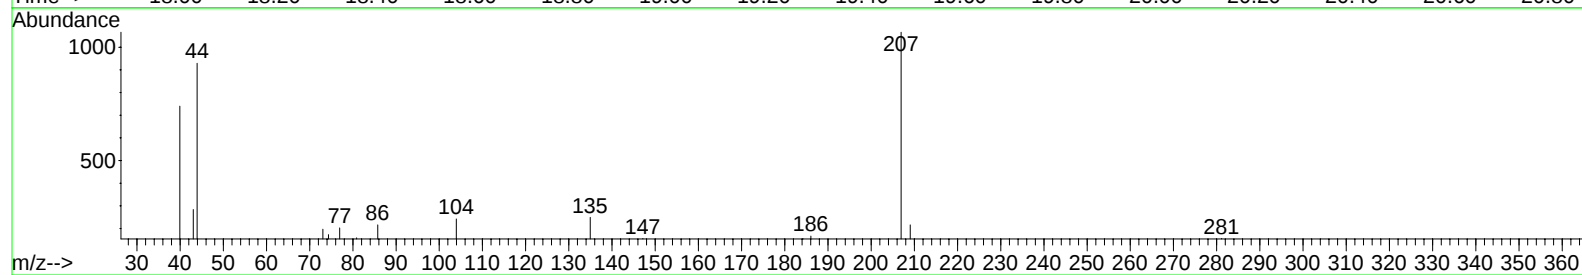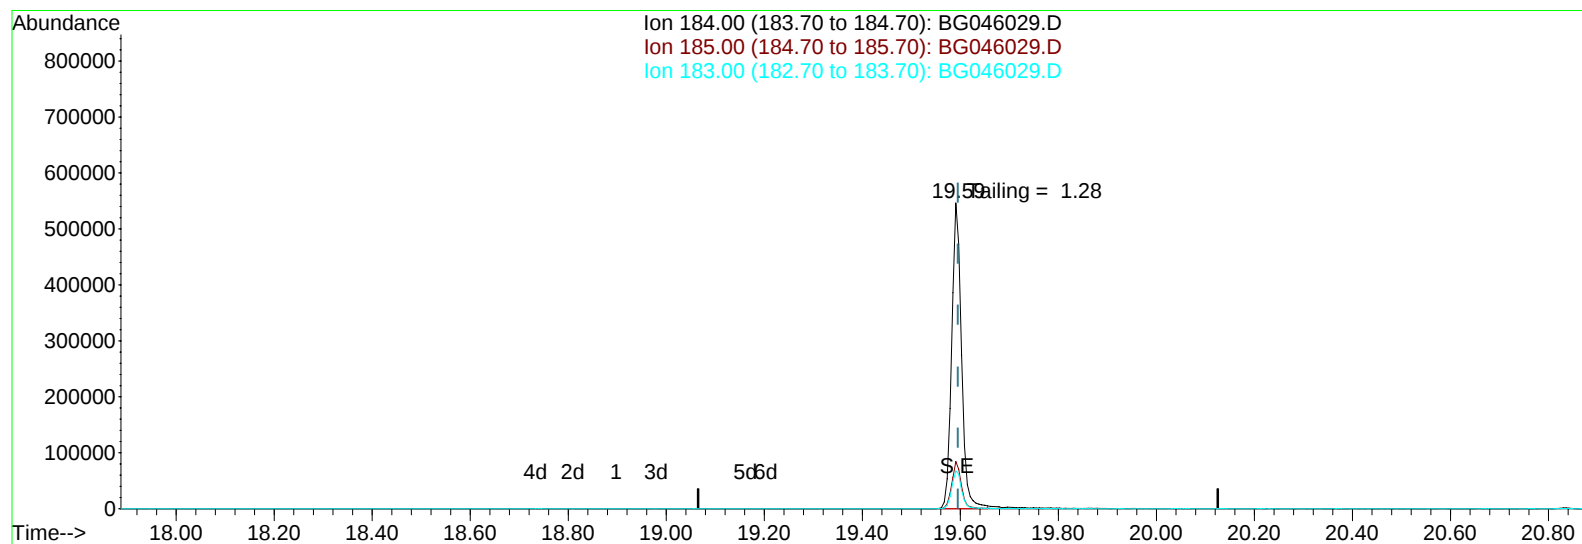

TIC: BG046029.D

(77) Benzidine

18.898min (-0.698) 0.36ng

response 54

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	0.00#
183.00	13.00	0.00#
0.00	0.00	0.00