


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071420\
 Data File : BG046029.D
 Acq On : 14 Jul 2020 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:58:53 2020

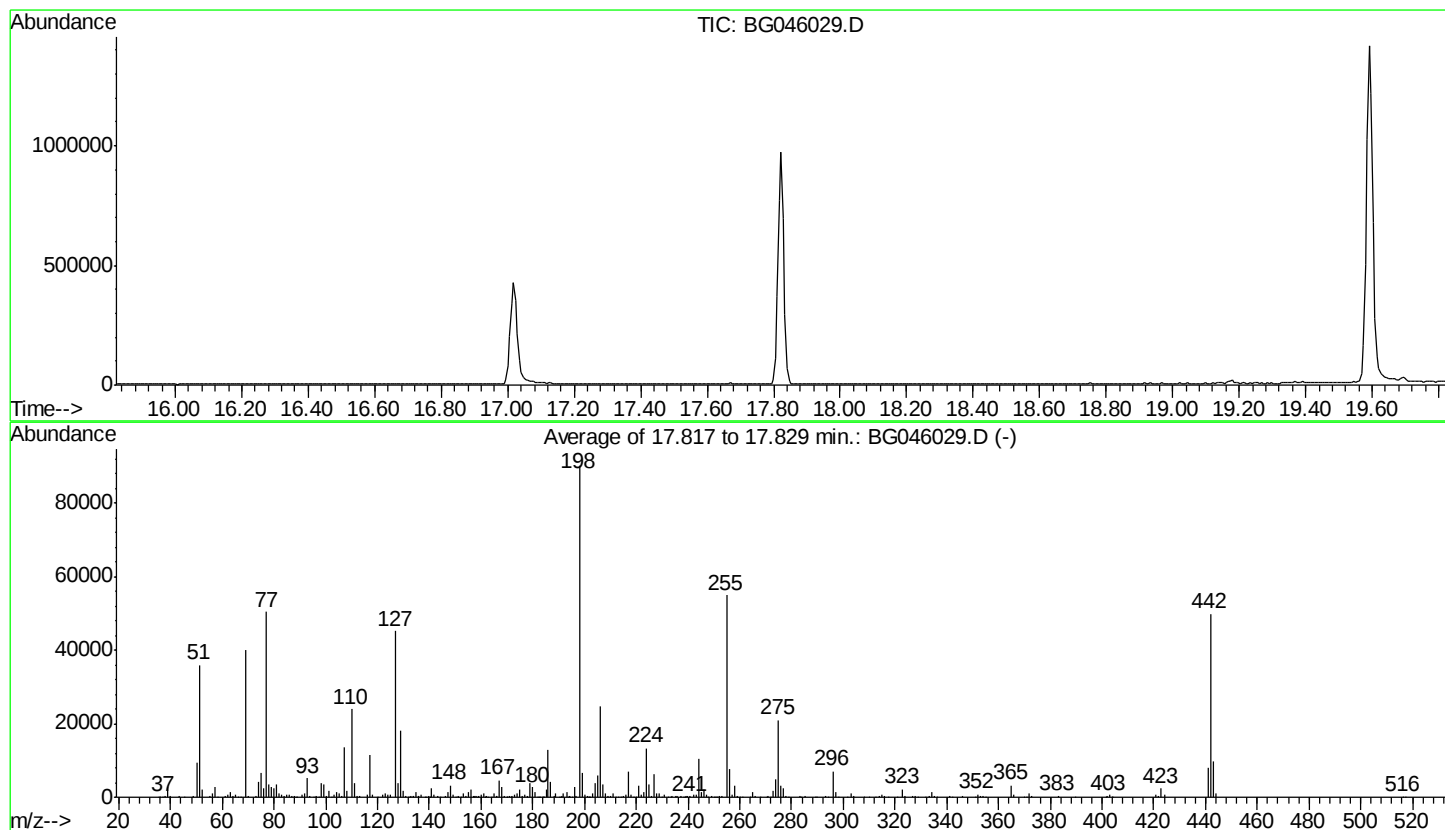

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	35978	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.5	40088	PASS
70	69	0.00	2	0.8	320	PASS
127	198	10	80	50.1	45125	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90101	PASS
199	198	5	9	7.2	6500	PASS
275	198	10	60	23.3	20962	PASS
365	198	1	100	3.6	3236	PASS
441	198	0.01	100	9.0	8071	PASS
442	198	50	100	55.3	49797	PASS
443	442	15	24	19.5	9722	PASS