

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
 Data File : BG049327.D
 Acq On : 14 Jul 2021 13:19
 Operator : CG/JU
 Sample : PB137664BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049327.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.109	7	12	22	rVB3	32154	71149	6.79%	0.703%
2	3.373	55	57	60	rBV2	1873	1443	0.14%	0.014%
3	3.455	68	71	77	rVB3	8651	11904	1.14%	0.118%
4	3.878	140	143	161	rBV	110654	212934	20.33%	2.103%
5	4.313	215	217	220	rBV2	1758	1579	0.15%	0.016%
6	4.448	236	240	242	rBV2	1818	2220	0.21%	0.022%
7	4.718	283	286	289	rBV3	1166	1581	0.15%	0.016%
8	4.989	326	332	333	rBV4	1047	1959	0.19%	0.019%
9	5.177	363	364	367	rBV2	1600	1658	0.16%	0.016%
10	5.247	372	376	380	rBV2	1358	2632	0.25%	0.026%
11	5.406	401	403	406	rVB2	1280	1422	0.14%	0.014%
12	5.559	425	429	430	rBV3	1516	1905	0.18%	0.019%
13	7.221	703	712	723	rBV	155276	275853	26.33%	2.725%
14	7.386	733	740	749	rBV	98734	172306	16.45%	1.702%
15	7.597	769	776	785	rVB	149665	264729	25.27%	2.615%
16	8.067	849	856	863	rBV	89215	157998	15.08%	1.560%
17	8.291	890	894	898	rBV3	954	1623	0.15%	0.016%
18	8.773	969	976	984	rBV2	184432	320786	30.62%	3.168%
19	9.231	1046	1054	1065	rBV	150192	276009	26.35%	2.726%
20	9.959	1171	1178	1188	rBV2	138435	249172	23.79%	2.461%
21	10.506	1264	1271	1282	rBV	178187	334368	31.92%	3.302%
22	10.888	1327	1336	1343	rBV	119391	217697	20.78%	2.150%
23	11.017	1351	1358	1372	rVB	176120	343229	32.77%	3.390%
24	12.474	1602	1606	1611	rVB2	2566	3160	0.30%	0.031%
25	13.326	1748	1751	1755	rBV2	1022	1776	0.17%	0.018%
26	14.113	1877	1885	1891	rBV	388066	586690	56.01%	5.795%
27	14.407	1928	1935	1943	rVB	386074	616507	58.86%	6.089%
28	14.713	1980	1987	1995	rBV	202748	320494	30.60%	3.165%
29	14.907	2014	2020	2032	rBV2	161516	284074	27.12%	2.806%
30	15.241	2072	2077	2078	rBV	1200	1941	0.19%	0.019%
31	15.706	2149	2156	2164	rVB	506593	774657	73.95%	7.651%
32	15.817	2169	2175	2184	rBV	160842	259930	24.81%	2.567%
33	15.946	2193	2197	2200	rVB4	5632	8224	0.79%	0.081%
34	16.487	2285	2289	2296	rBV3	2312	3596	0.34%	0.036%
35	17.257	2419	2420	2423	rVB2	2250	1581	0.15%	0.016%
36	17.368	2436	2439	2442	rVB	1105	1570	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
 Data File : BG049327.D
 Acq On : 14 Jul 2021 13:19
 Operator : CG/JU
 Sample : PB137664BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

37	17.462	2448	2455	2462	rBV	271698	418284	39.93%	4.131%
38	17.562	2465	2472	2479	rBV	571823	875091	83.54%	8.643%
39	18.784	2678	2680	2686	rBV3	1346	1970	0.19%	0.019%
40	18.902	2699	2700	2704	rVB2	1351	1425	0.14%	0.014%
41	19.290	2760	2766	2771	rBV5	1191	2628	0.25%	0.026%
42	19.419	2786	2788	2789	rBV2	2511	1450	0.14%	0.014%
43	19.483	2795	2799	2805	rVB2	7134	8802	0.84%	0.087%
44	19.583	2811	2816	2818	rBV3	1310	2439	0.23%	0.024%
45	19.742	2836	2843	2847	rBV3	6002	10763	1.03%	0.106%
46	19.848	2854	2861	2867	rBV	721783	1047497	100.00%	10.346%
47	20.259	2929	2931	2932	rBV2	2655	1631	0.16%	0.016%
48	20.294	2935	2937	2939	rBV3	2848	2195	0.21%	0.022%
49	20.606	2988	2990	2991	rBV2	3630	2438	0.23%	0.024%
50	20.835	3027	3029	3031	rBV3	3264	3176	0.30%	0.031%
51	21.746	3177	3184	3191	rBV	264547	452973	43.24%	4.474%
52	24.807	3695	3705	3715	rVB	360058	1014503	96.85%	10.020%
53	25.030	3734	3743	3755	rVB2	161891	487280	46.52%	4.813%




Sum of corrected areas: 10124901

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049327.D
Acq On : 14 Jul 2021 13:19
Operator : CG/JU
Sample : PB137664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK664

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

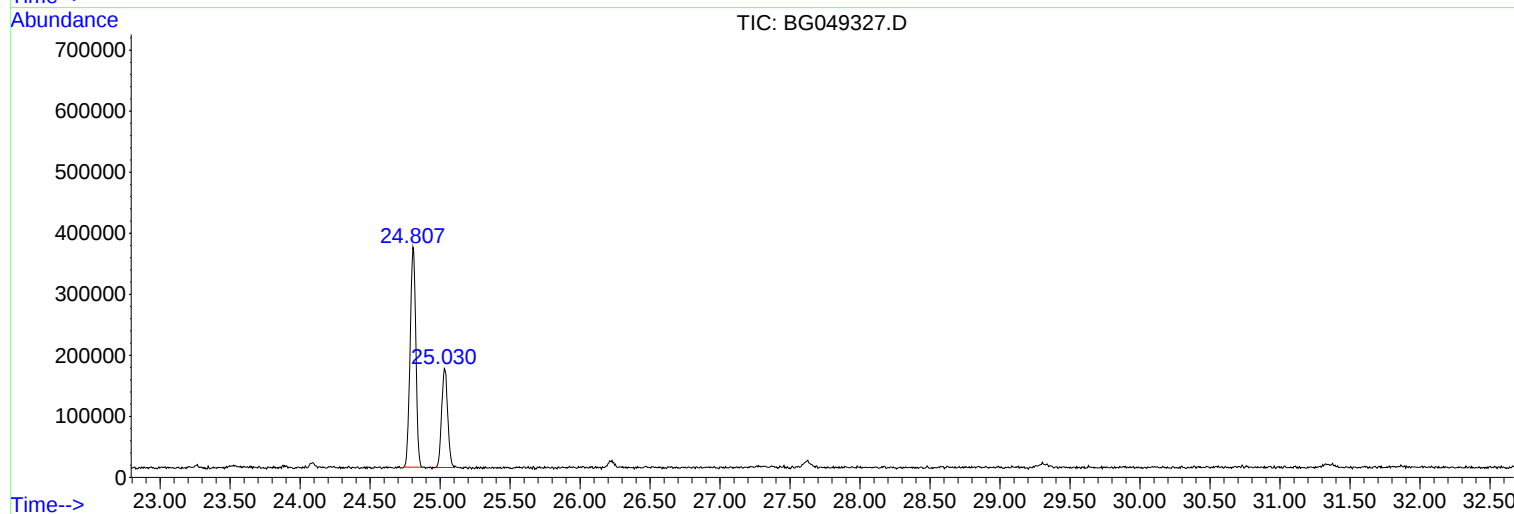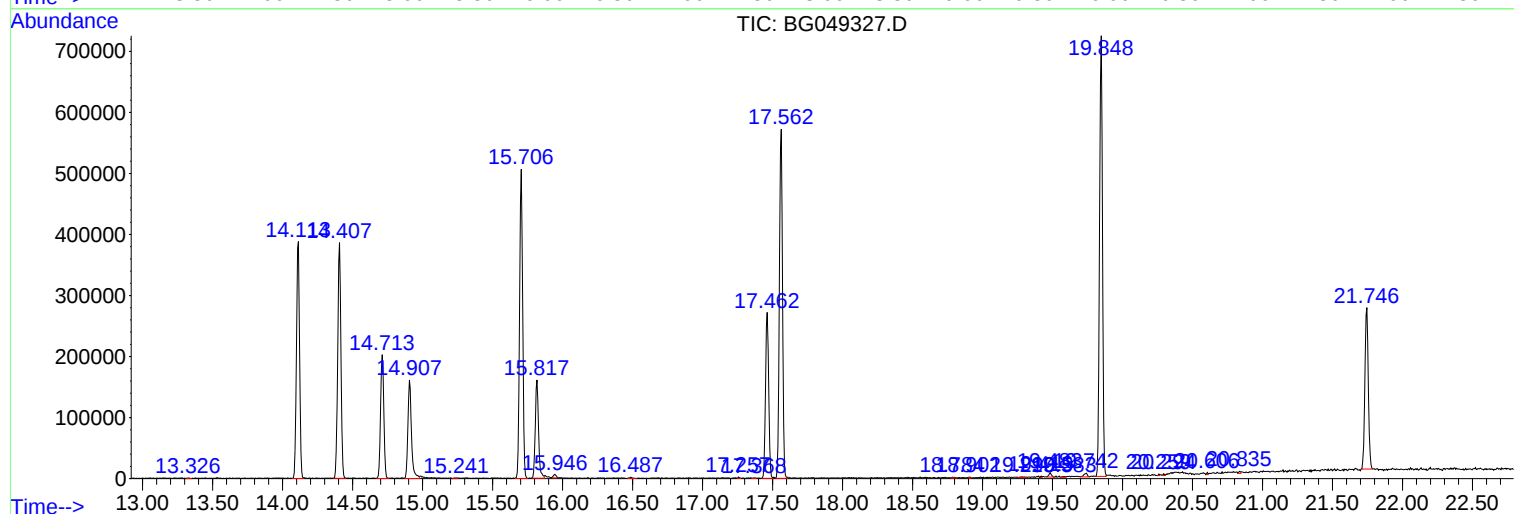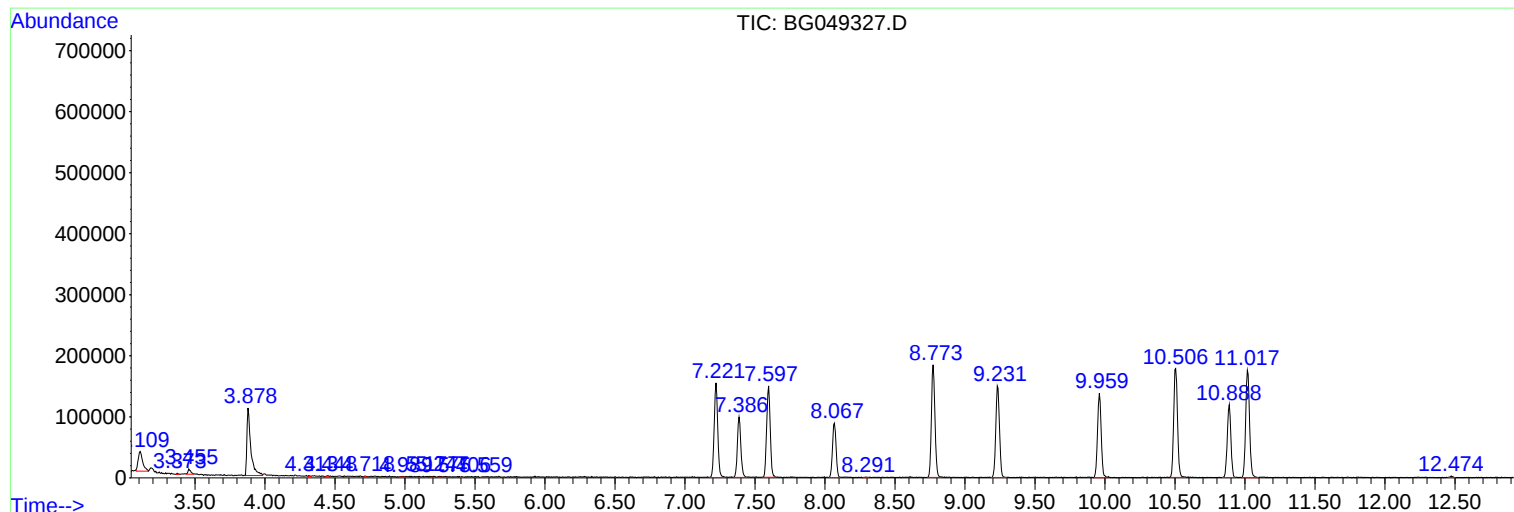

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049327.D
Acq On : 14 Jul 2021 13:19
Operator : CG/JU
Sample : PB137664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK664









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.11 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.110	9.01 ng/ul	71149	1,4-Dichlorobenzene-d4	8.062

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	87
2			Cyclohexane	84	C6H12	000110-82-7	87
3			Cyclohexane	84	C6H12	000110-82-7	83
4			Cyclohexane	84	C6H12	000110-82-7	80
5			Cyclohexane	84	C6H12	000110-82-7	64

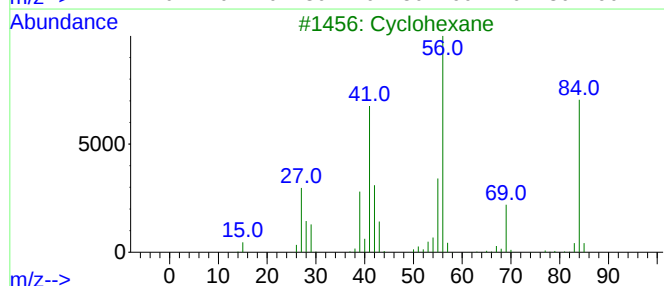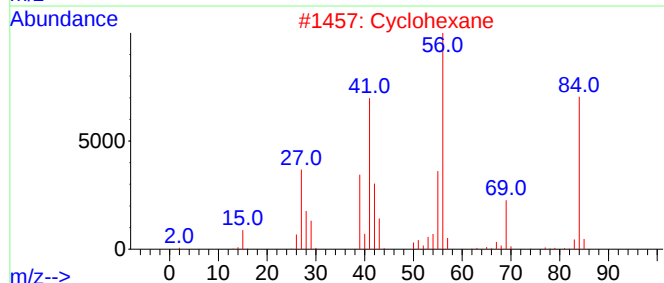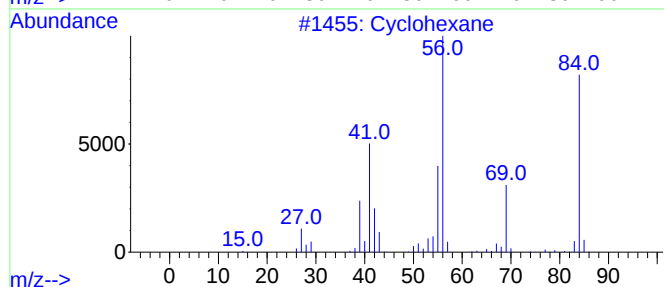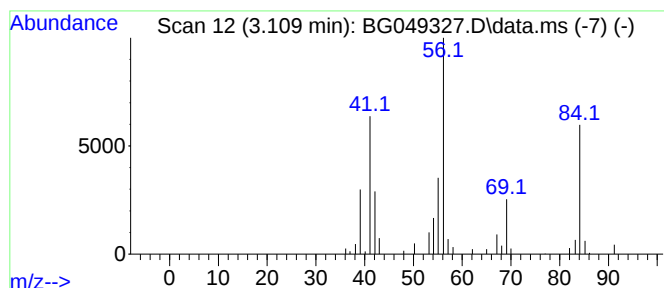

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049327.D
Acq On : 14 Jul 2021 13:19
Operator : CG/JU
Sample : PB137664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK664

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.110	9.0	ng/ul	71149	1	8.062	157998	20.0