

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
 Data File : BG049356.D
 Acq On : 15 Jul 2021 10:34
 Operator : CG/JU
 Sample : PB137619BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049356.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.107	7	12	22	rVB4	32082	76350	6.77%	0.654%
2	3.454	68	71	79	rVB3	11194	18196	1.61%	0.156%
3	3.877	140	143	154	rBV	121304	220988	19.58%	1.894%
4	4.429	234	237	239	rBV2	1634	1788	0.16%	0.015%
5	5.140	356	358	361	rBV3	1800	1720	0.15%	0.015%
6	5.698	450	453	455	rBV2	1682	1892	0.17%	0.016%
7	6.950	663	666	669	rBV2	1223	1659	0.15%	0.014%
8	7.026	677	679	685	rVB3	938	1597	0.14%	0.014%
9	7.085	687	689	693	rBV4	1367	2107	0.19%	0.018%
10	7.220	705	712	722	rBV	191082	335305	29.71%	2.874%
11	7.385	733	740	749	rBV	113409	195622	17.34%	1.677%
12	7.596	769	776	784	rBV	173956	314648	27.88%	2.697%
13	8.066	849	856	863	rVB	115064	201895	17.89%	1.731%
14	8.389	908	911	916	rBV3	1659	1958	0.17%	0.017%
15	8.771	968	976	985	rBV	228042	399106	35.37%	3.421%
16	9.229	1046	1054	1064	rBV	177886	324054	28.72%	2.778%
17	9.429	1085	1088	1091	rBV2	1356	1995	0.18%	0.017%
18	9.958	1170	1178	1187	rBV	166000	305296	27.06%	2.617%
19	10.181	1212	1216	1219	rBV2	1148	1635	0.14%	0.014%
20	10.499	1263	1270	1282	rVB	234389	431782	38.26%	3.701%
21	10.645	1291	1295	1296	rBV	1483	1860	0.16%	0.016%
22	10.880	1328	1335	1345	rVB	152242	283491	25.12%	2.430%
23	11.016	1349	1358	1369	rBV	216837	405734	35.96%	3.478%
24	12.050	1533	1534	1539	rBV2	1397	1793	0.16%	0.015%
25	12.473	1599	1606	1612	rBV6	3128	5706	0.51%	0.049%
26	14.106	1878	1884	1891	rBV	426886	634480	56.23%	5.438%
27	14.406	1928	1935	1941	rBV	431250	697574	61.82%	5.979%
28	14.711	1980	1987	1996	rVB	254808	402605	35.68%	3.451%
29	14.905	2014	2020	2030	rBV	189344	325239	28.82%	2.788%
30	15.222	2071	2074	2079	rBV2	1399	2119	0.19%	0.018%
31	15.704	2149	2156	2163	rBV	549814	856260	75.88%	7.339%
32	15.816	2168	2175	2186	rBV	172097	275409	24.41%	2.361%
33	15.939	2193	2196	2201	rVB2	6284	7775	0.69%	0.067%
34	16.121	2226	2227	2233	rVB2	1482	1811	0.16%	0.016%
35	16.486	2287	2289	2292	rVB2	2268	2192	0.19%	0.019%
36	16.580	2302	2305	2307	rBV	1563	1582	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
 Data File : BG049356.D
 Acq On : 15 Jul 2021 10:34
 Operator : CG/JU
 Sample : PB137619BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK619

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
 Title : SVOA CALIBRATION

37	16.785	2337	2340	2344	rBV2	1033	1876	0.17%	0.016%
38	16.973	2367	2372	2373	rBV2	1344	1627	0.14%	0.014%
39	17.461	2448	2455	2462	rVB	338670	502583	44.54%	4.308%
40	17.561	2465	2472	2481	rVB	643651	960212	85.09%	8.230%
41	19.482	2795	2799	2806	rVB	8199	13194	1.17%	0.113%
42	19.735	2839	2842	2849	rVB2	5839	7898	0.70%	0.068%
43	19.846	2853	2861	2867	rBV	803279	1124295	99.64%	9.637%
44	20.034	2892	2893	2896	rBV3	2391	1622	0.14%	0.014%
45	20.087	2900	2902	2905	rBV2	1991	2181	0.19%	0.019%
46	20.240	2926	2928	2930	rBV2	2125	2010	0.18%	0.017%
47	20.587	2985	2987	2990	rBV2	2126	2198	0.19%	0.019%
48	20.869	3033	3035	3037	rBV2	2819	2408	0.21%	0.021%
49	21.339	3113	3115	3116	rBV	3291	1931	0.17%	0.017%
50	21.356	3116	3118	3119	rBV2	3274	1963	0.17%	0.017%
51	21.503	3142	3143	3145	rBV2	3313	1831	0.16%	0.016%
52	21.744	3177	3184	3195	rVV2	332281	561592	49.77%	4.814%
53	21.844	3199	3201	3203	rBV3	4405	3089	0.27%	0.026%
54	24.805	3695	3705	3715	rVB	403429	1128411	100.00%	9.672%
55	25.034	3734	3744	3756	rVB2	209039	598678	53.05%	5.132%
56	28.195	4281	4282	4283	rBV	3985	1901	0.17%	0.016%




Sum of corrected areas: 11666723

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049356.D
Acq On : 15 Jul 2021 10:34
Operator : CG/JU
Sample : PB137619BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK619

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

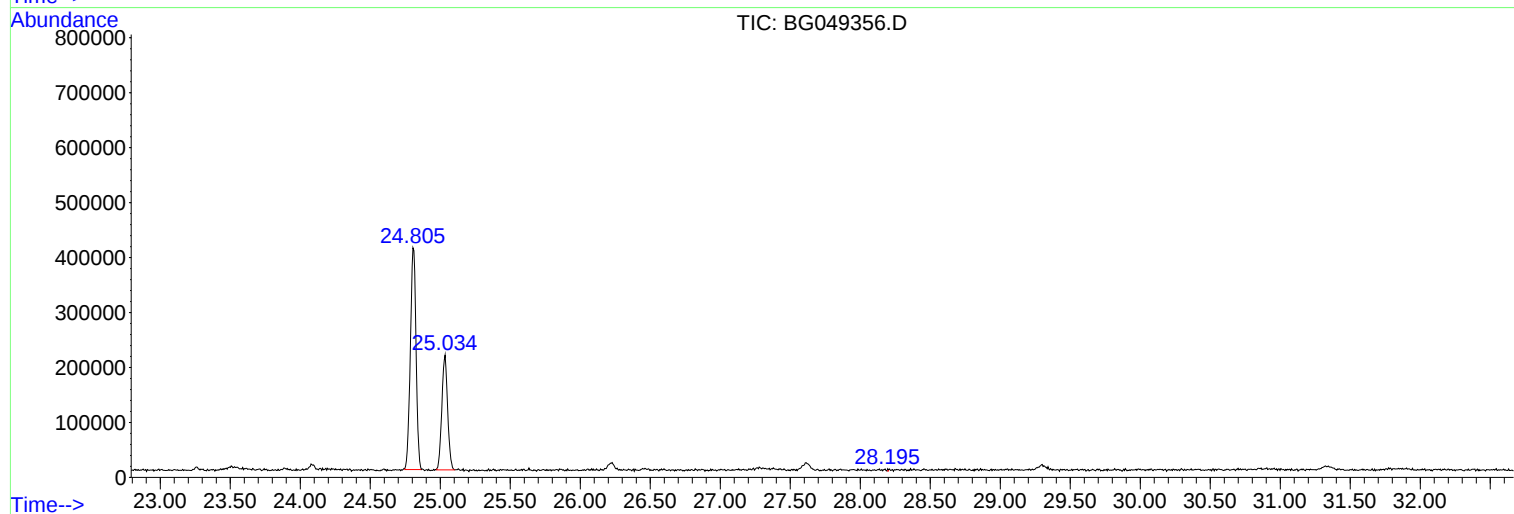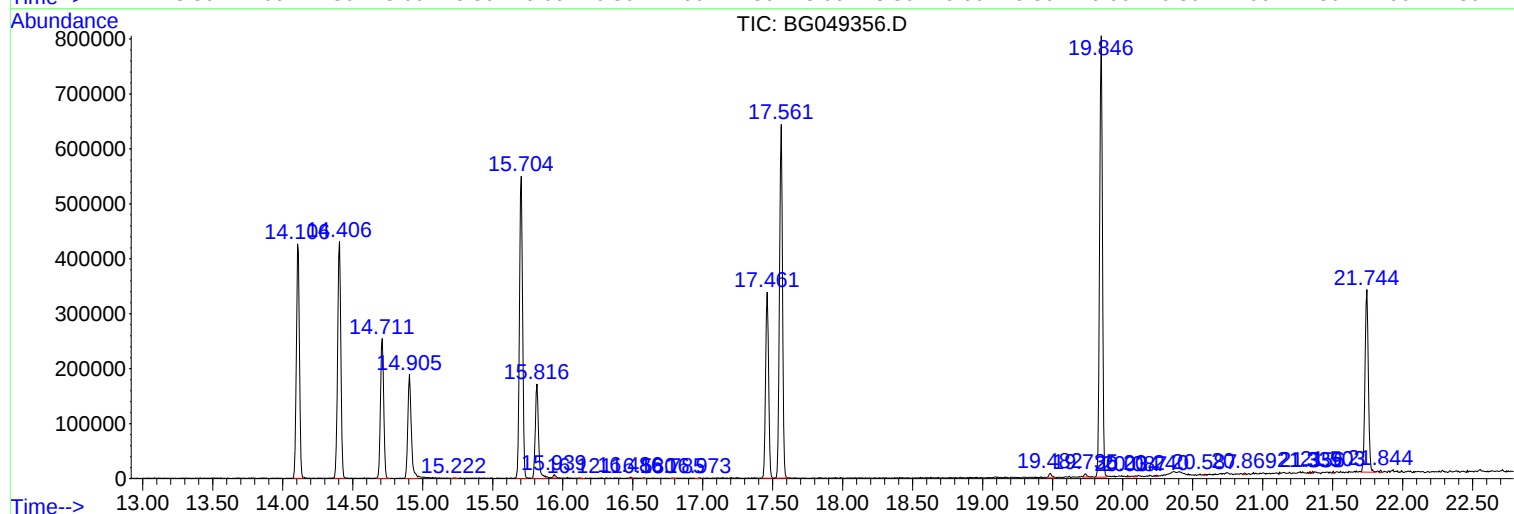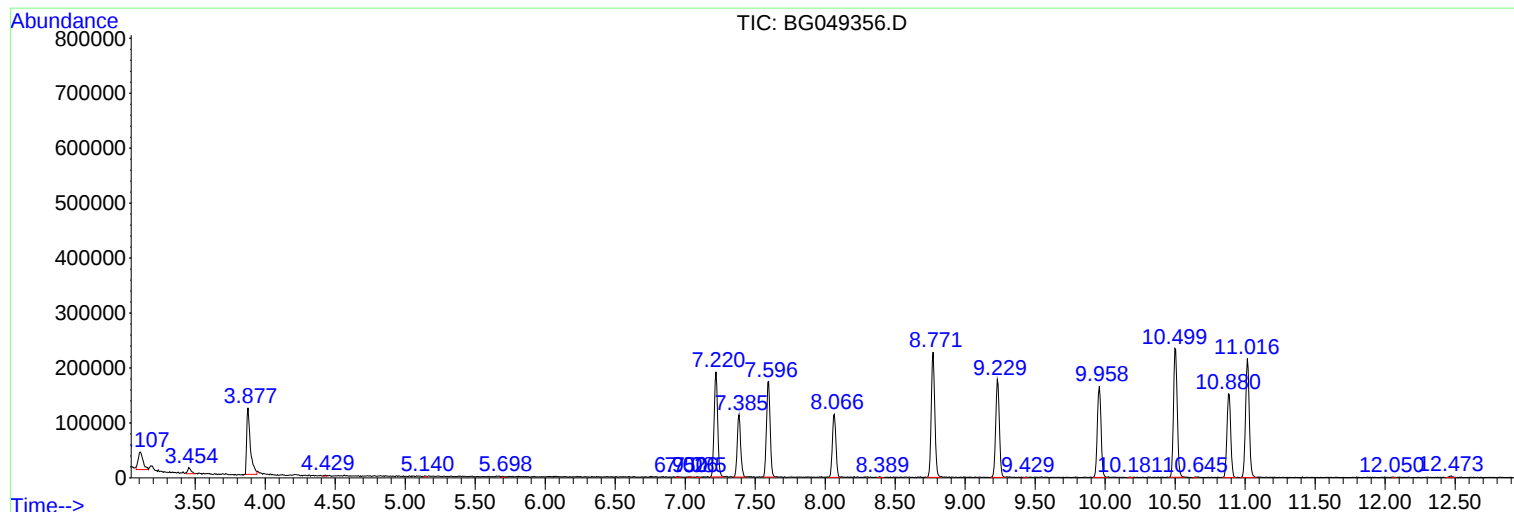

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049356.D
Acq On : 15 Jul 2021 10:34
Operator : CG/JU
Sample : PB137619BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK619

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071421\
Data File : BG049356.D
Acq On : 15 Jul 2021 10:34
Operator : CG/JU
Sample : PB137619BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK619

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG070921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
