
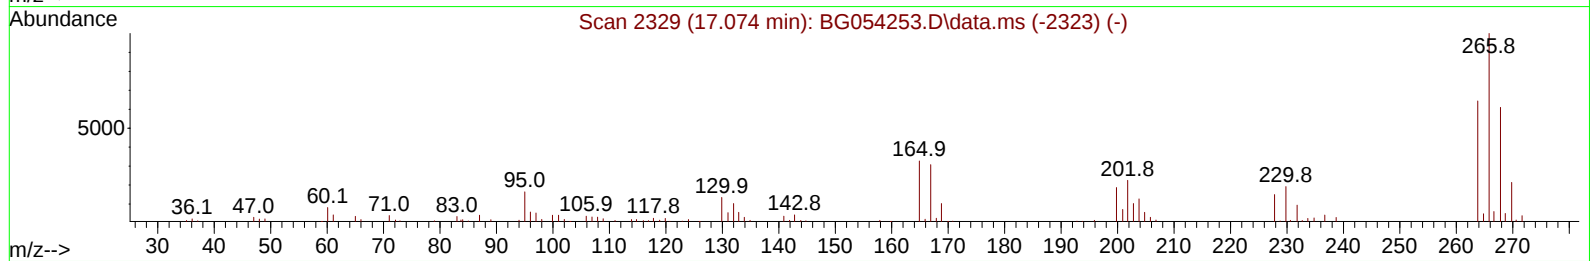
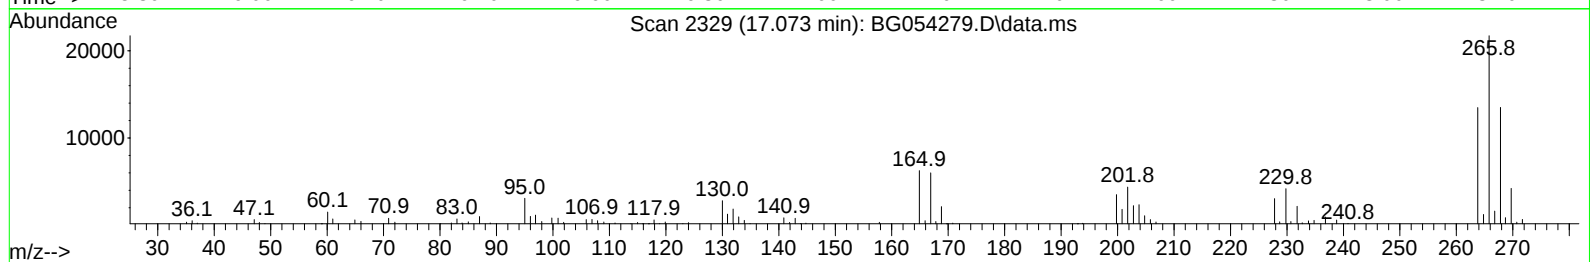


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054279.D
Acq On : 14 Jul 2022 13:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:30:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

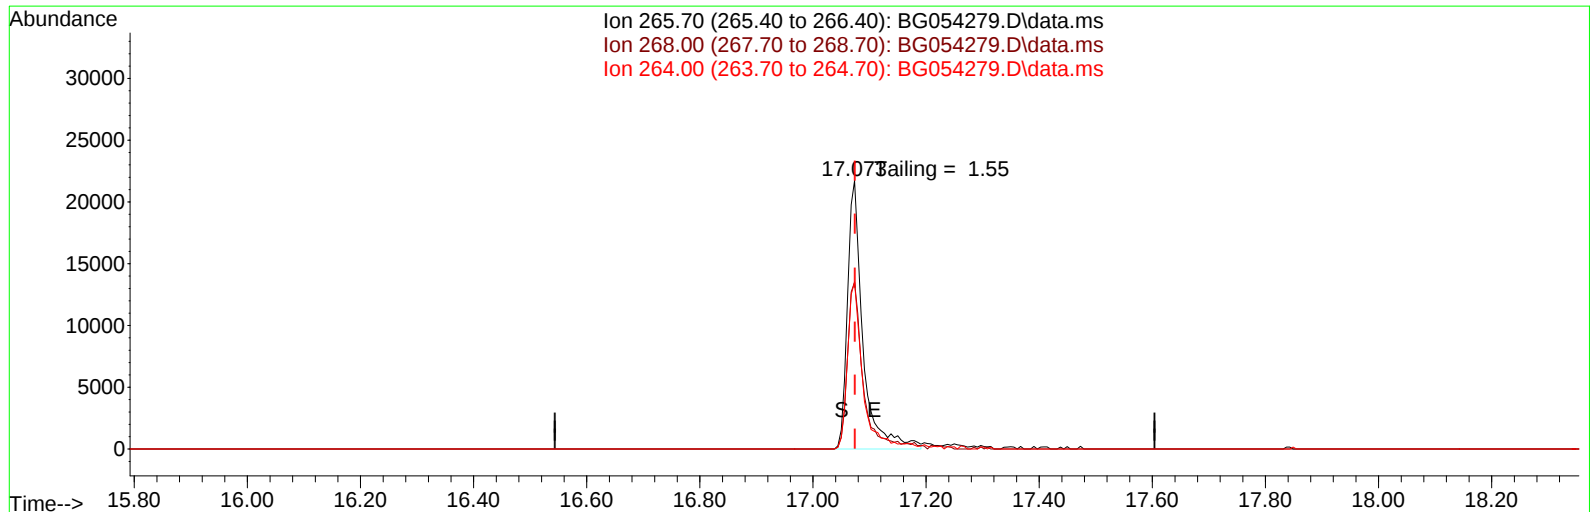

TIC: BG054279.D\data.ms

(70) Pentachlorophenol (C)




17.073min (-0.001) 18420.62 ng

response 38965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	66.14
264.00	66.20	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054279.D
Acq On : 14 Jul 2022 13:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 05:30:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

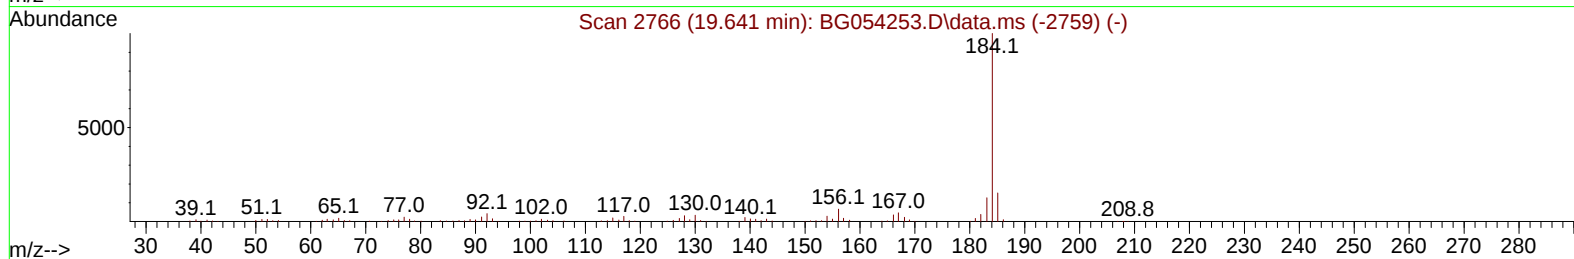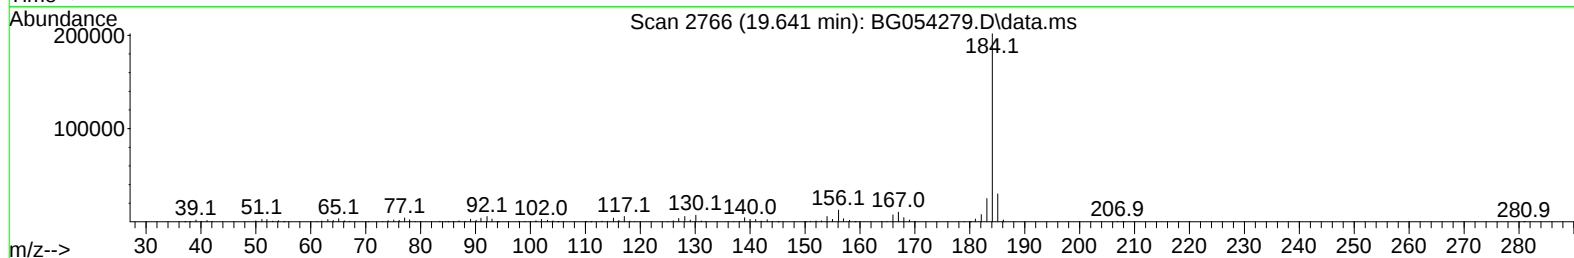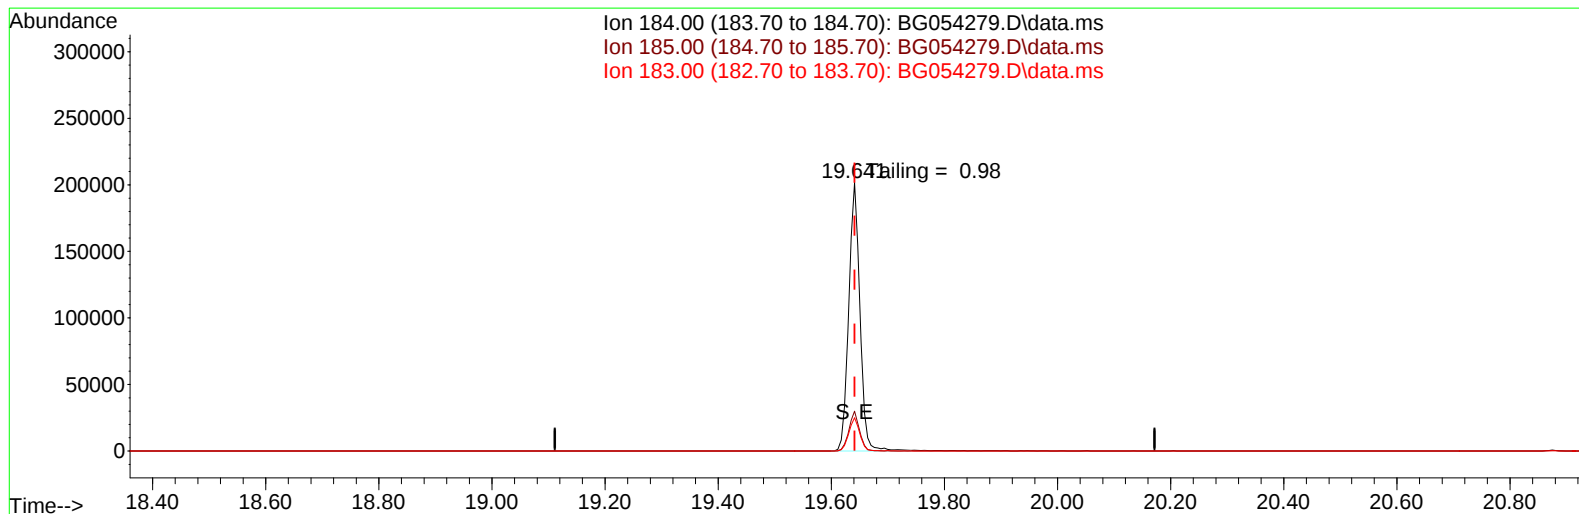

TIC: BG054279.D\data.ms

(77) Benzidine

19.641min (-0.000) 0.00 ng

response 278874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.84
183.00	11.10	12.42
0.00	0.00	0.00