

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
 Data File : BG054287.D
 Acq On : 14 Jul 2022 19:45
 Operator : CG/JU
 Sample : N3711-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PSC124019

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.610	371	378	388	rBV	210083	351224	23.20%	5.531%
2	7.208	642	650	665	rBB	221052	395533	26.12%	6.229%
3	8.036	785	791	801	rVB	52898	91274	6.03%	1.437%
4	9.199	981	989	999	rBV2	132903	248546	16.42%	3.914%
5	10.845	1262	1269	1277	rBV	71693	130512	8.62%	2.055%
6	13.289	1678	1685	1692	rBV	464414	731246	48.30%	11.515%
7	14.664	1913	1919	1927	rBB	130612	217382	14.36%	3.423%
8	16.150	2166	2172	2189	rBV2	462030	747897	49.40%	11.777%
9	17.407	2380	2386	2391	rBV	202011	319089	21.08%	5.025%
10	17.449	2391	2393	2399	rVB	15342	20868	1.38%	0.329%
11	19.458	2731	2735	2743	rVB	51961	76259	5.04%	1.201%
12	19.822	2793	2797	2805	rVB	57963	84776	5.60%	1.335%
13	20.016	2824	2830	2836	rBV	1130023	1514062	100.00%	23.843%
14	20.316	2878	2881	2886	rVB2	11471	15358	1.01%	0.242%
15	21.315	3045	3051	3056	rBV4	21381	38992	2.58%	0.614%
16	21.679	3105	3113	3119	rBV2	273182	515121	34.02%	8.112%
17	21.726	3119	3121	3128	rVB	31485	42281	2.79%	0.666%
18	22.408	3233	3237	3243	rVB5	8351	16583	1.10%	0.261%
19	22.478	3243	3249	3258	rBV10	8254	22316	1.47%	0.351%
20	22.854	3306	3313	3319	rVB6	8478	19090	1.26%	0.301%
21	23.882	3478	3488	3496	rBV	29250	96517	6.37%	1.520%
22	24.617	3603	3613	3619	rBV	15856	44134	2.91%	0.695%
23	24.758	3627	3637	3651	rVB2	19971	60174	3.97%	0.948%
24	24.910	3651	3663	3676	rBV2	156468	472417	31.20%	7.439%
25	28.606	4279	4292	4297	rBV4	10317	37872	2.50%	0.596%
26	29.758	4475	4488	4498	rBV3	8240	40725	2.69%	0.641%




Sum of corrected areas: 6350248

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054287.D
Acq On : 14 Jul 2022 19:45
Operator : CG/JU
Sample : N3711-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC124019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

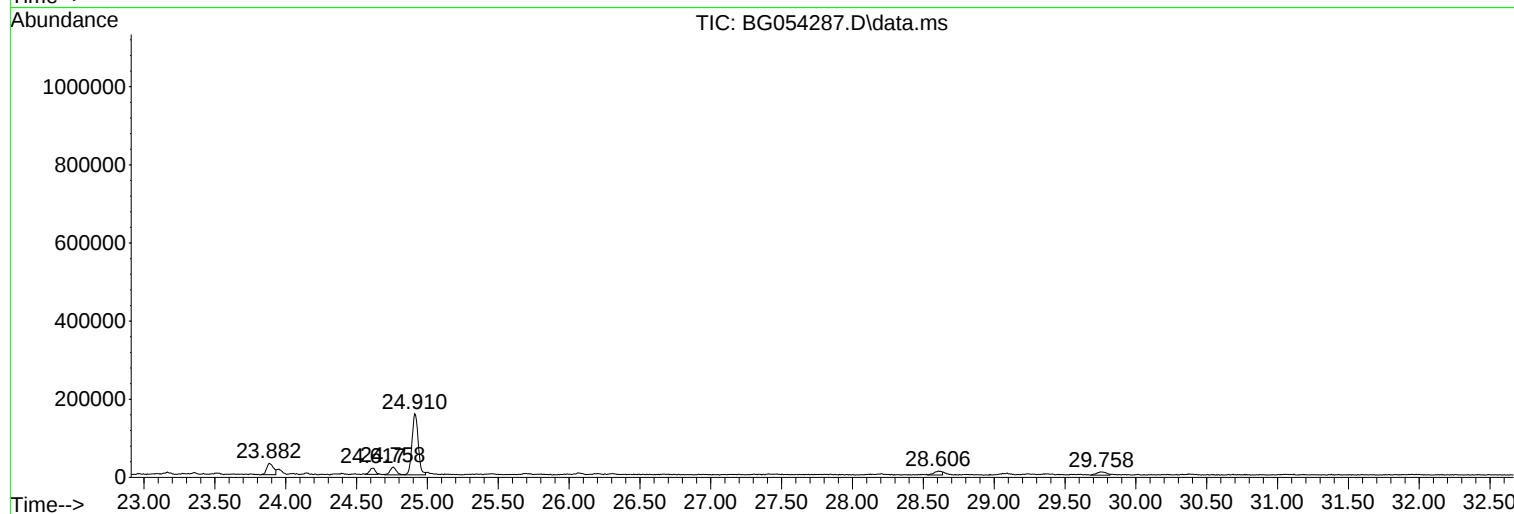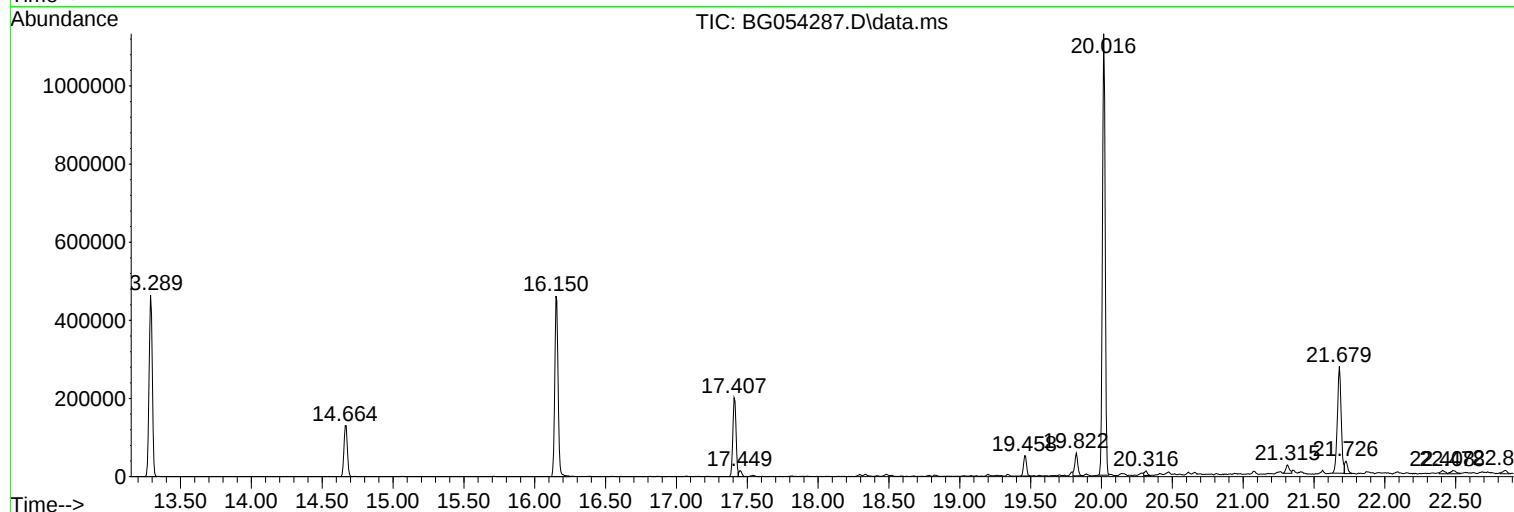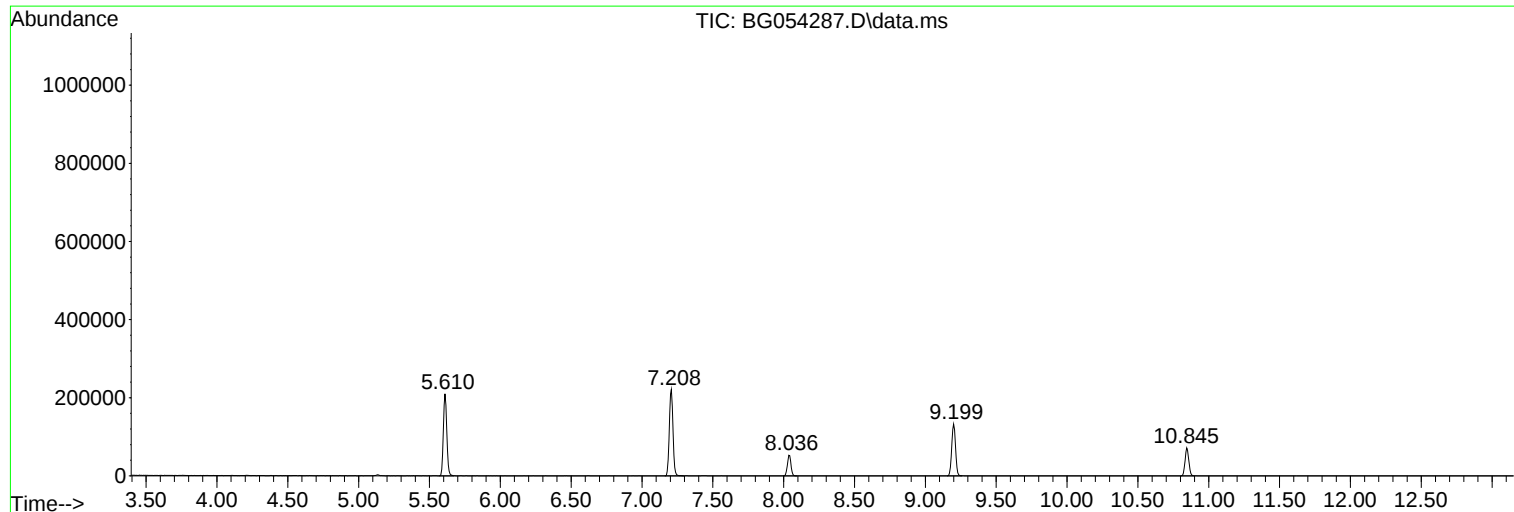

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054287.D
Acq On : 14 Jul 2022 19:45
Operator : CG/JU
Sample : N3711-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC124019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054287.D
Acq On : 14 Jul 2022 19:45
Operator : CG/JU
Sample : N3711-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PSC124019

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------