
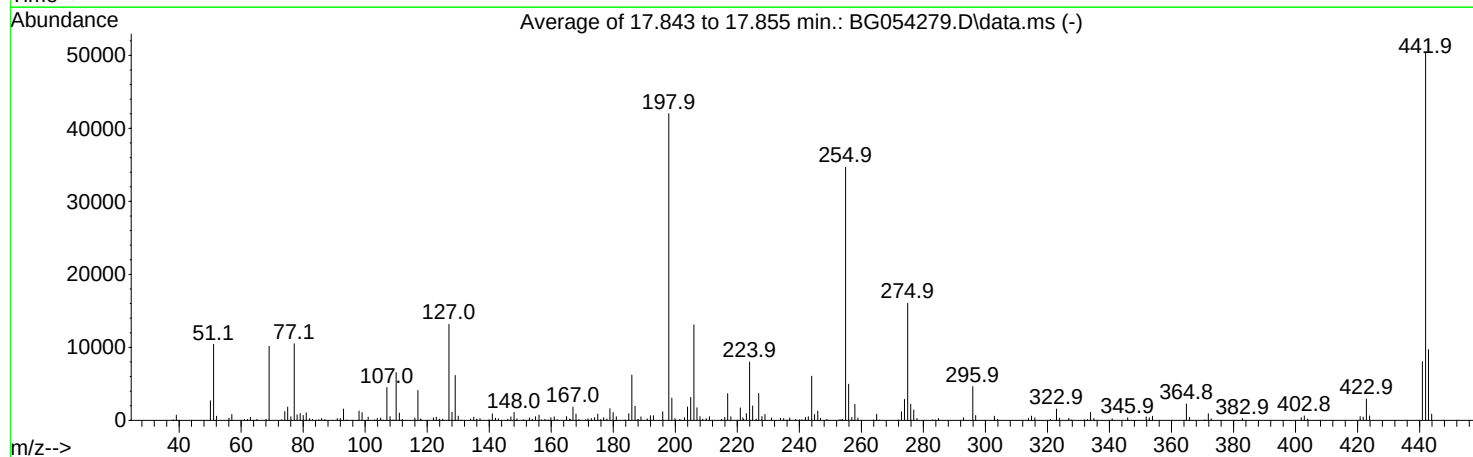


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
 Data File : BG054279.D
 Acq On : 14 Jul 2022 13:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 15:49:20 2022

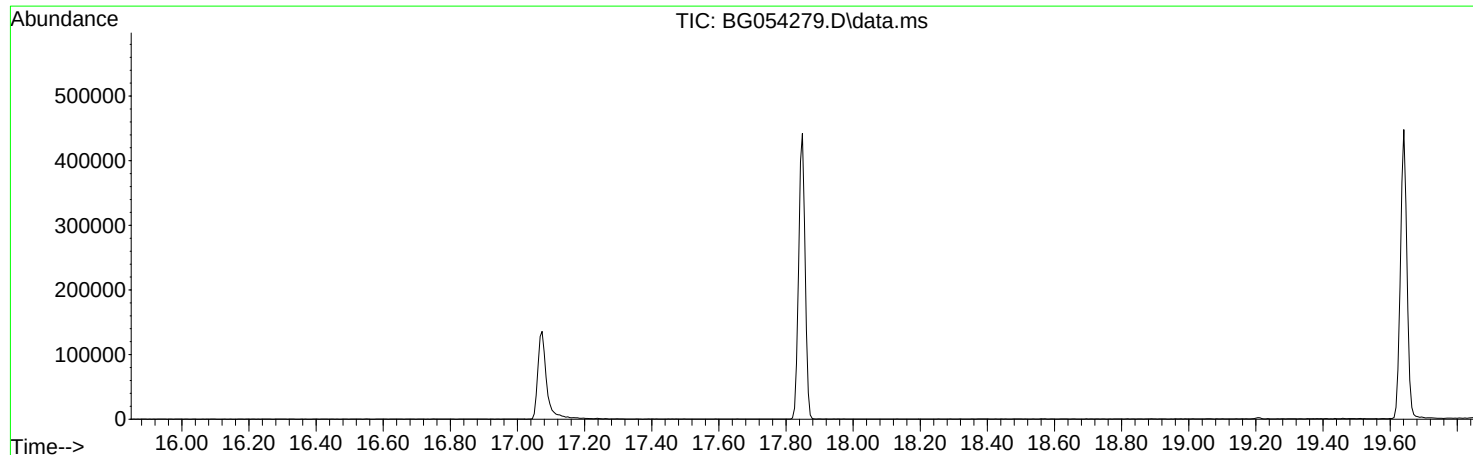




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	10405	PASS
68	69	0.00	2	1.6	158	PASS
69	198	0.00	100	24.2	10153	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.3	13154	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42019	PASS
199	198	5	9	7.3	3049	PASS
275	198	10	60	38.2	16037	PASS
365	198	1	100	5.3	2248	PASS
441	198	0.01	100	19.1	8034	PASS
442	442	50	100	100.0	50392	PASS
443	442	15	24	19.2	9680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054279.D
Acq On : 14 Jul 2022 13:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 15 05:30:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

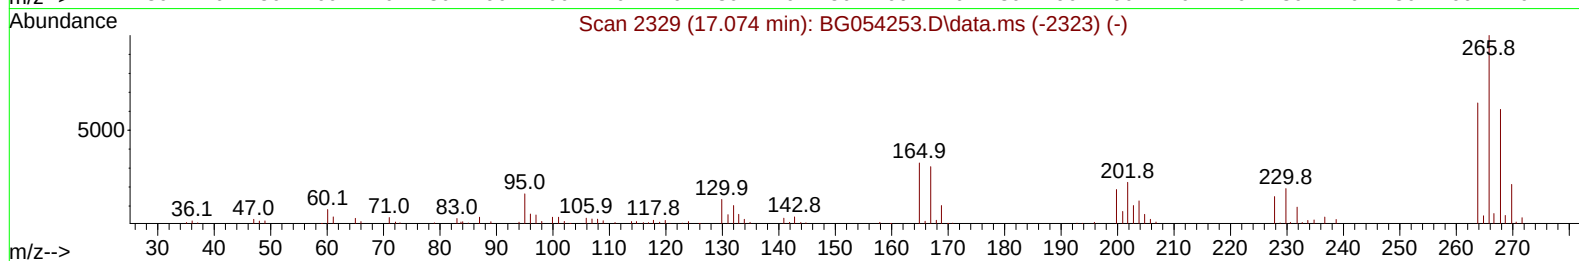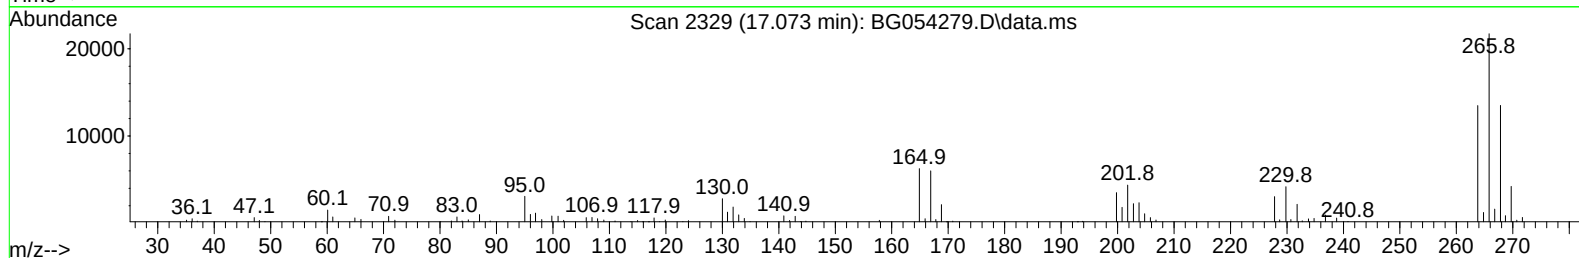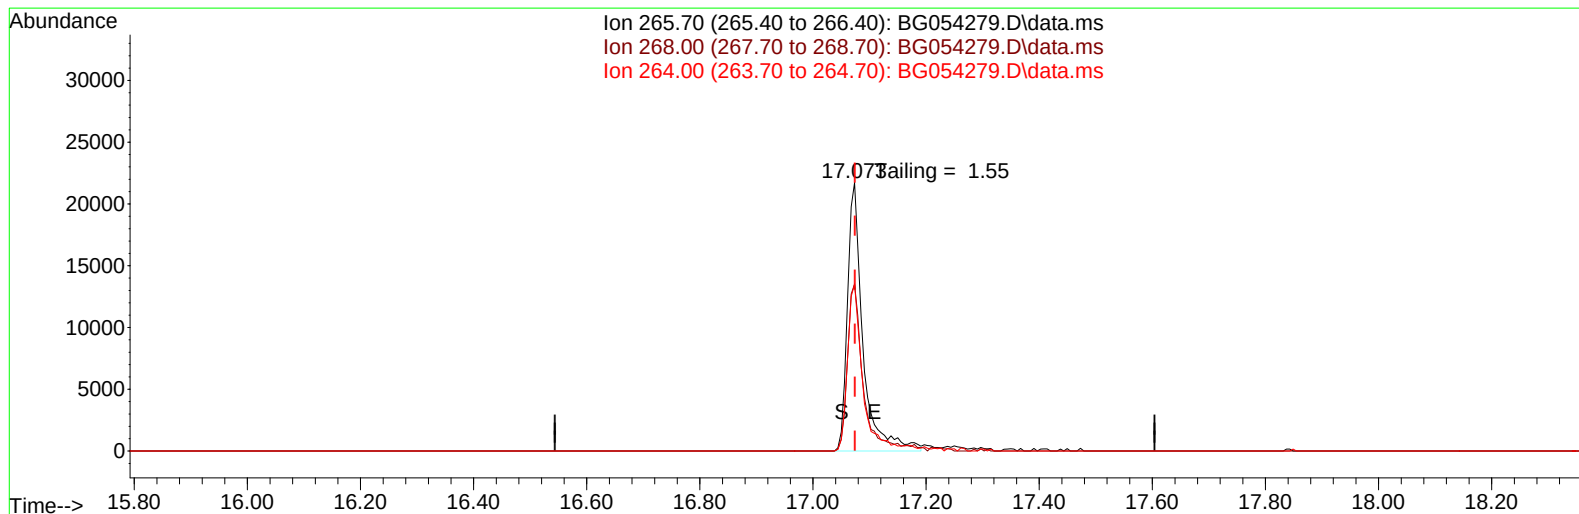

TIC: BG054279.D\data.ms

(70) Pentachlorophenol (C)

17.073min (-0.001) 18420.62 ng




response 38965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	66.14
264.00	66.20	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071422\
Data File : BG054279.D
Acq On : 14 Jul 2022 13:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 15 05:30:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 15:49:20 2022
Response via : Initial Calibration

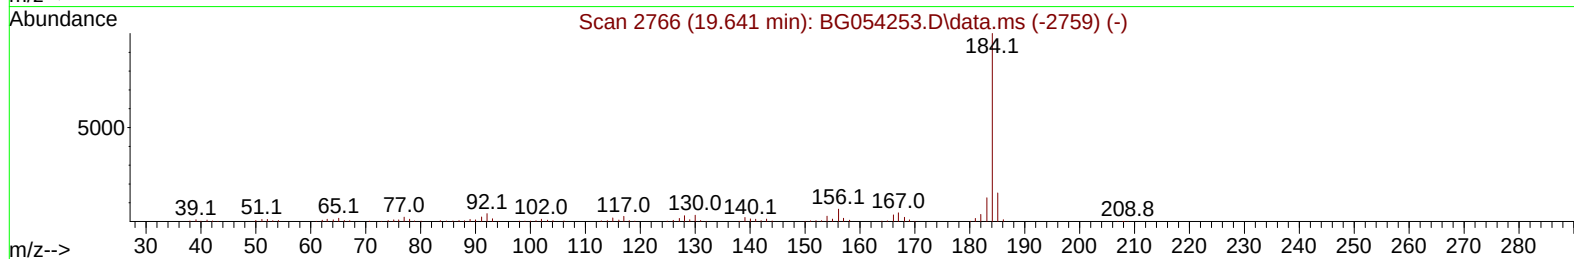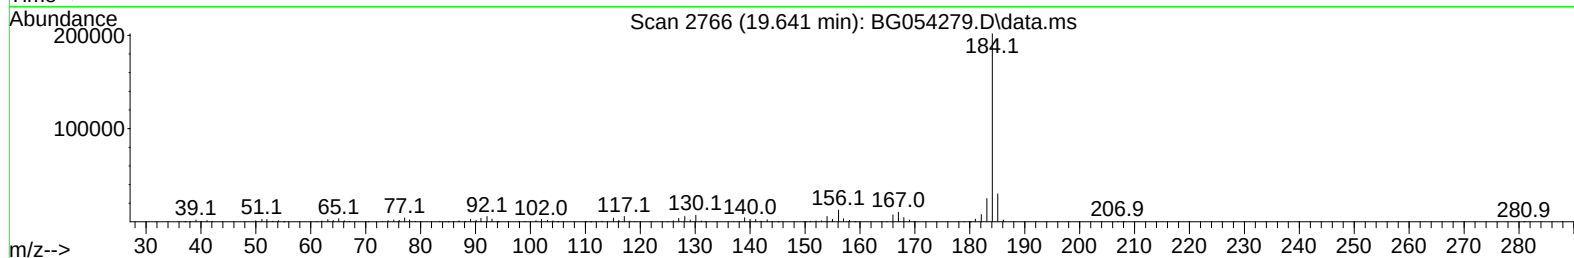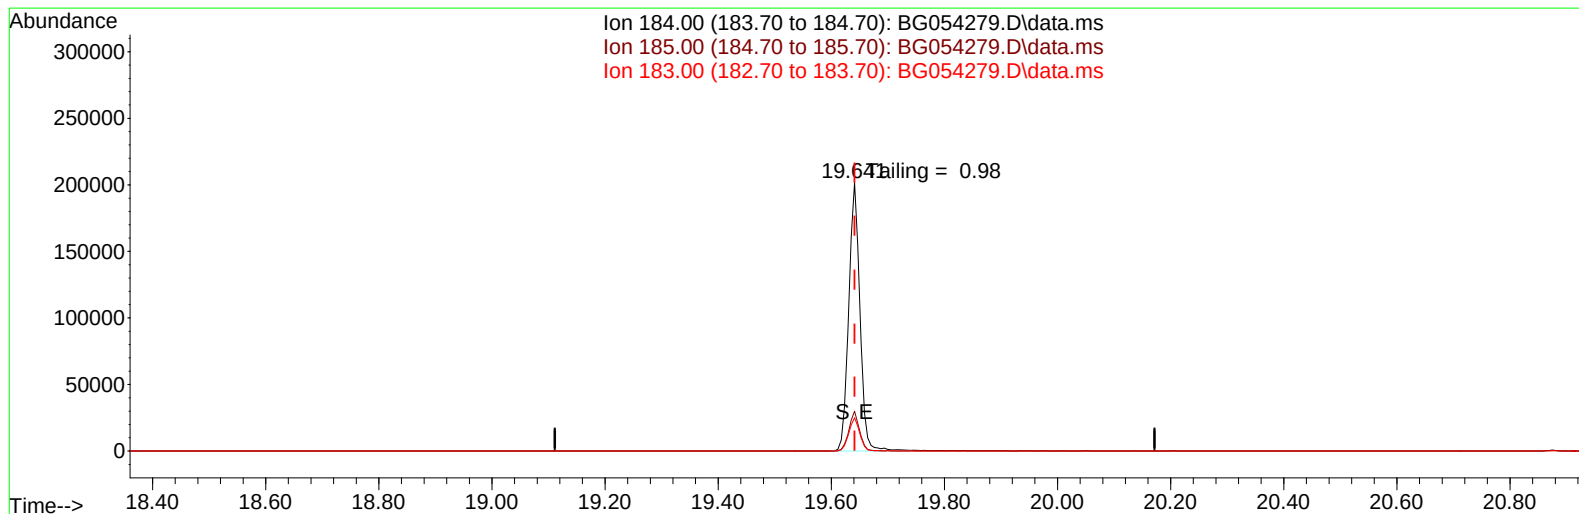

TIC: BG054279.D\data.ms

(77) Benzidine

19.641min (-0.000) 0.00 ng

response 278874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.84
183.00	11.10	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2022	BNA_G	<u>BG054279.D</u>
Compound Name	Response	Retention Time
DDT	171069	20.875
DDD	9557	20.434
DDE	0	19.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9557	180626	5.29

Instrument :
BNA_G
ClientSampleId :
DFTPP