
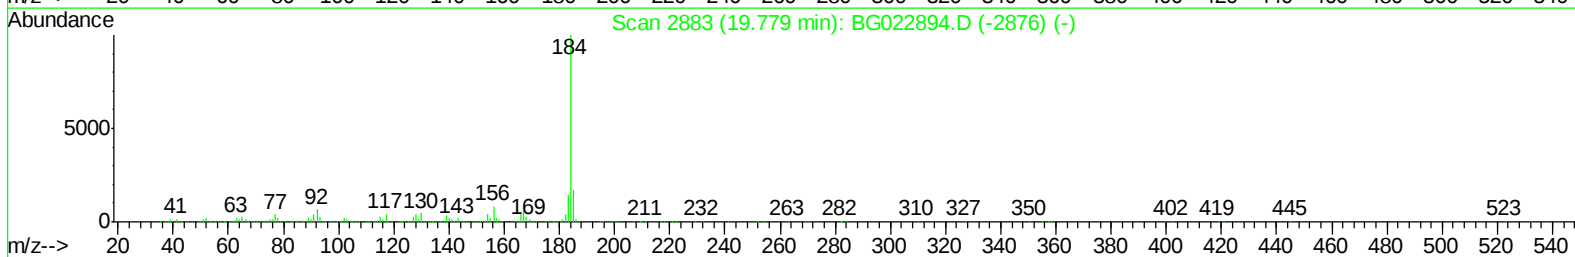
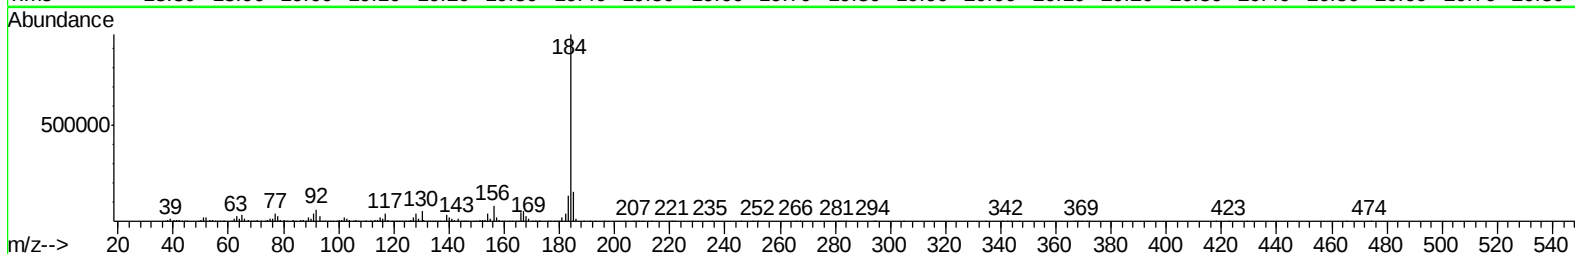


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071516\
Data File : BG023126.D
Acq On : 16 Jul 2016 00:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 07:00:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

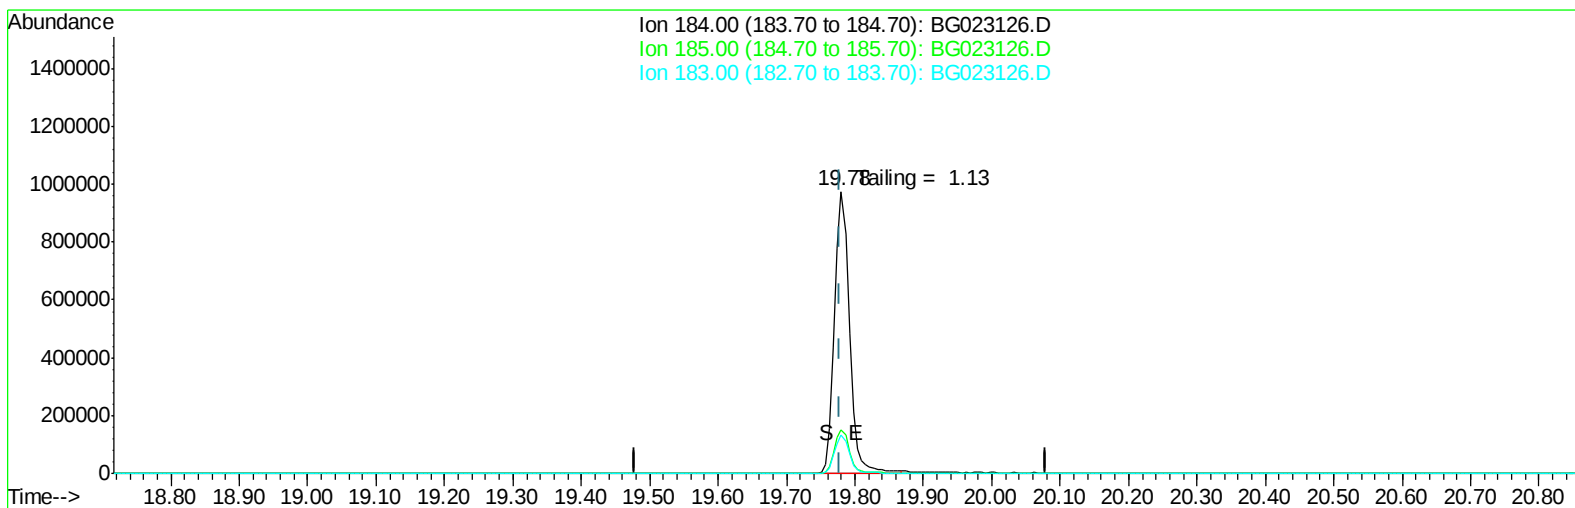

TIC: BG023126.D

(76) Benzidine




19.780min (+0.001) 25811.04ng

response 1464394

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.68
183.00	13.40	13.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071516\
Data File : BG023126.D
Acq On : 16 Jul 2016 00:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 07:00:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

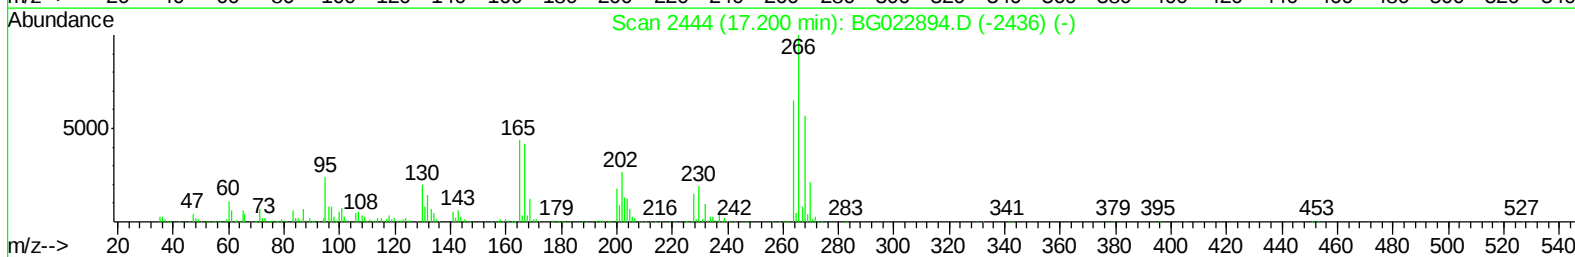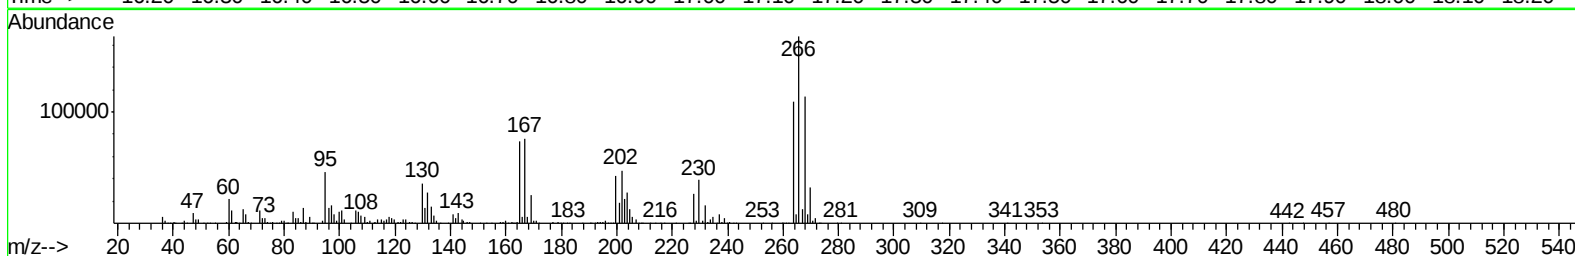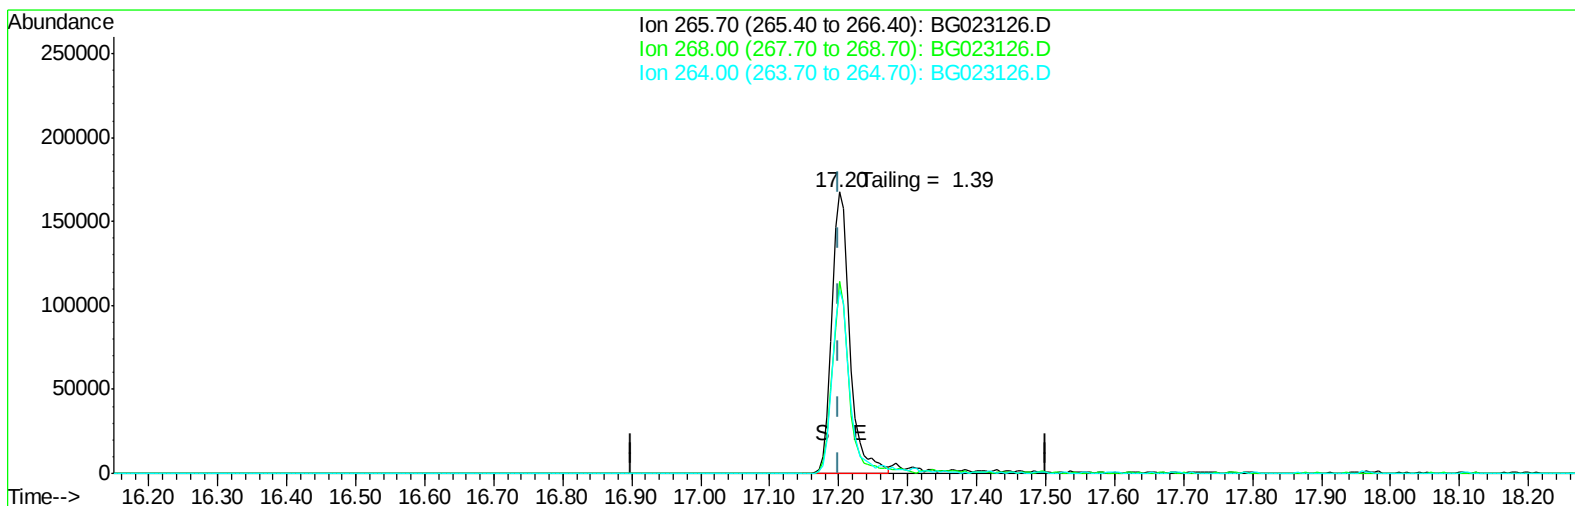

TIC: BG023126.D

(69) Pentachlorophenol (C)

17.201min (+0.001) 30084.38ng

response 306193

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	68.03
264.00	63.20	64.85
0.00	0.00	0.00