


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071516\
 Data File : BG023110.D
 Acq On : 15 Jul 2016 12:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

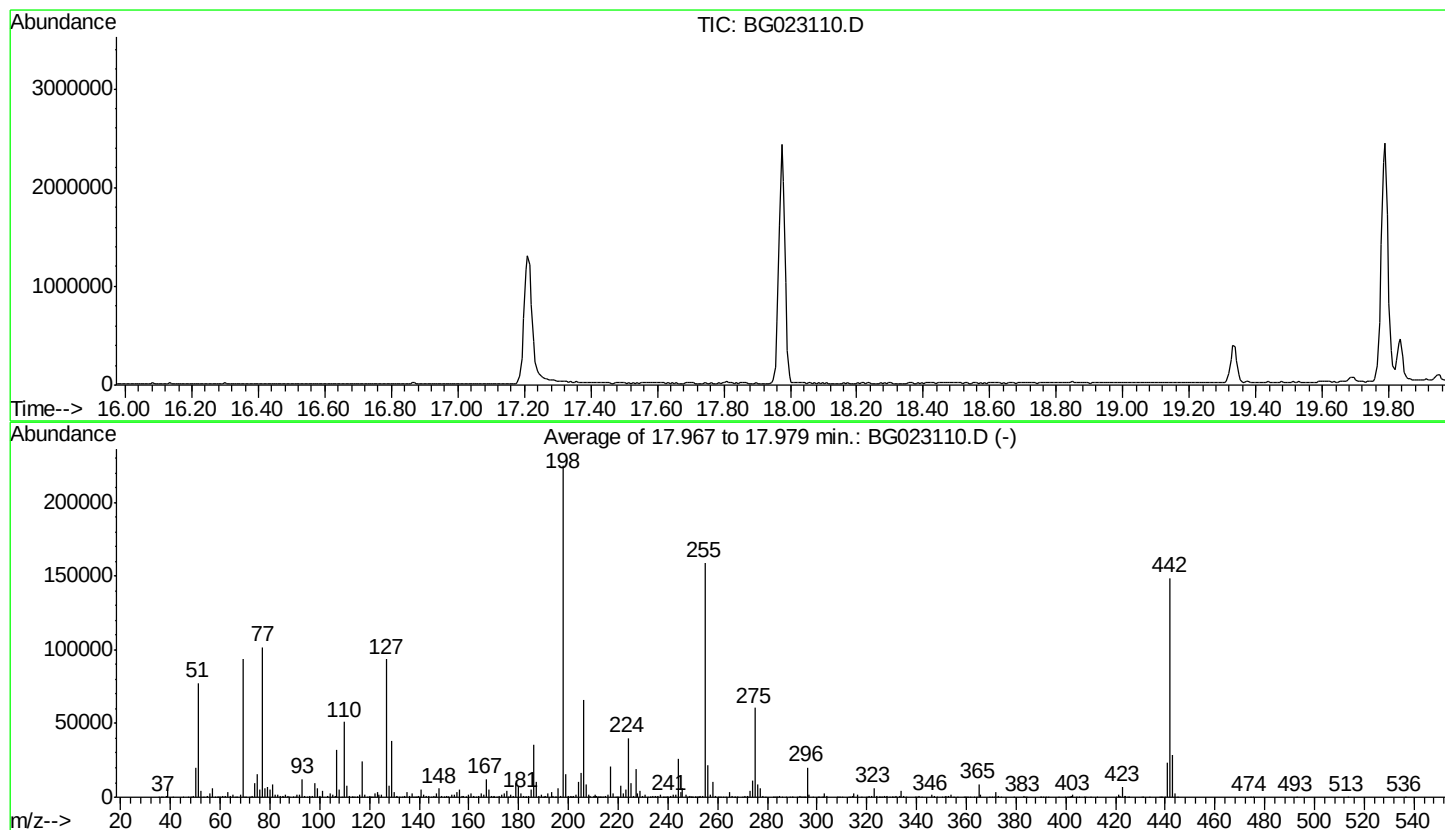

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	77658	PASS
68	69	0.00	2	1.7	1566	PASS
69	198	0.00	100	41.7	93800	PASS
70	69	0.00	2	0.4	419	PASS
127	198	10	80	41.5	93376	PASS
197	198	0.00	2	0.3	624	PASS
198	198	100	100	100.0	224810	PASS
199	198	5	9	7.0	15797	PASS
275	198	10	60	26.9	60456	PASS
365	198	1	100	3.9	8835	PASS
441	442	0.01	24	15.8	23444	PASS
442	198	50	100	66.2	148829	PASS
443	442	15	24	19.1	28357	PASS