


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071516\
 Data File : BG023126.D
 Acq On : 16 Jul 2016 00:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

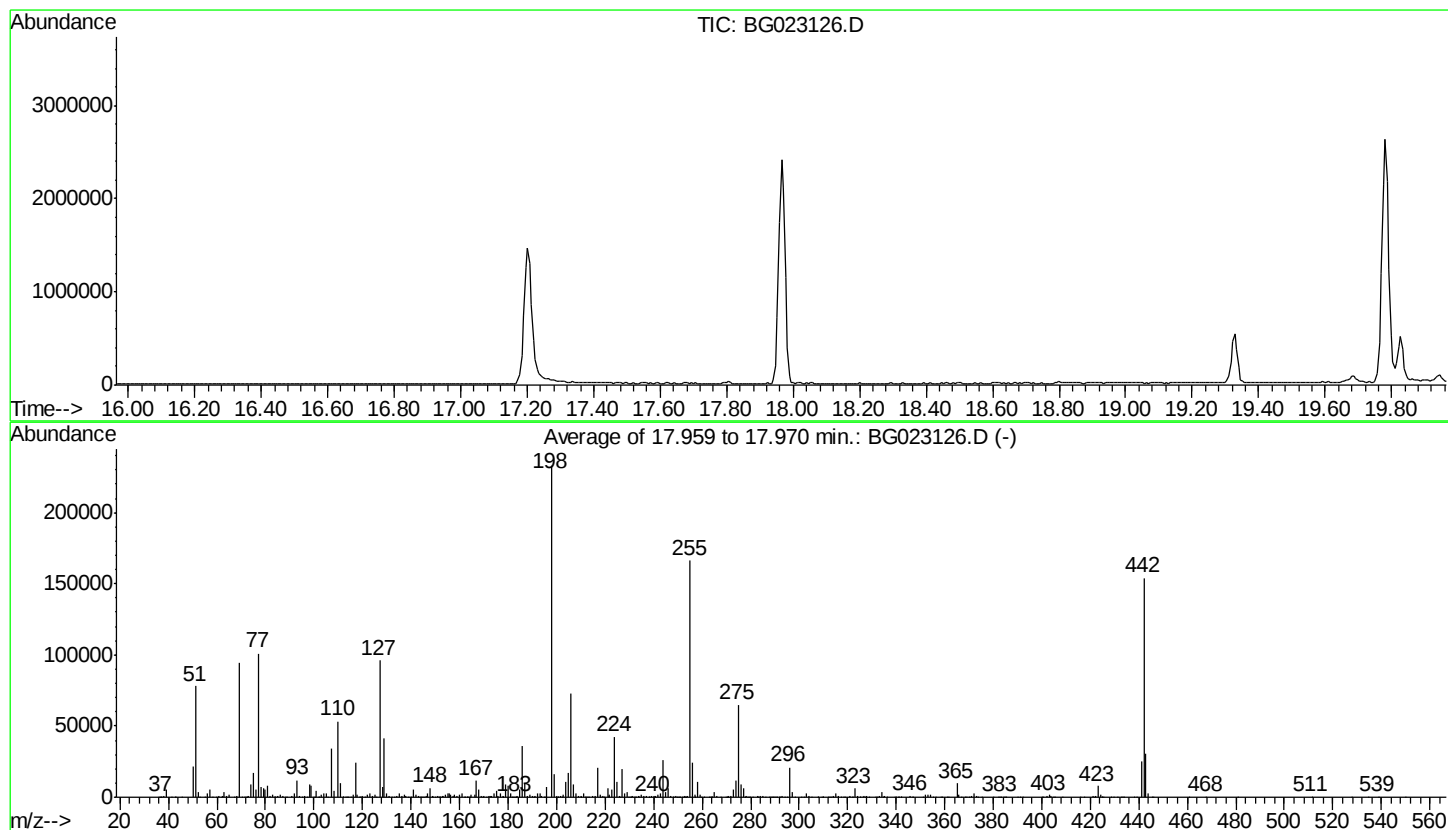

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	78017	PASS
68	69	0.00	2	0.7	656	PASS
69	198	0.00	100	40.4	94026	PASS
70	69	0.00	2	0.5	433	PASS
127	198	10	80	41.3	96184	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	232981	PASS
199	198	5	9	7.0	16337	PASS
275	198	10	60	27.9	64920	PASS
365	198	1	100	4.1	9512	PASS
441	442	0.01	24	16.1	24885	PASS
442	198	50	100	66.2	154189	PASS
443	442	15	24	19.7	30325	PASS