


Benzaldehyde


Response Ratio

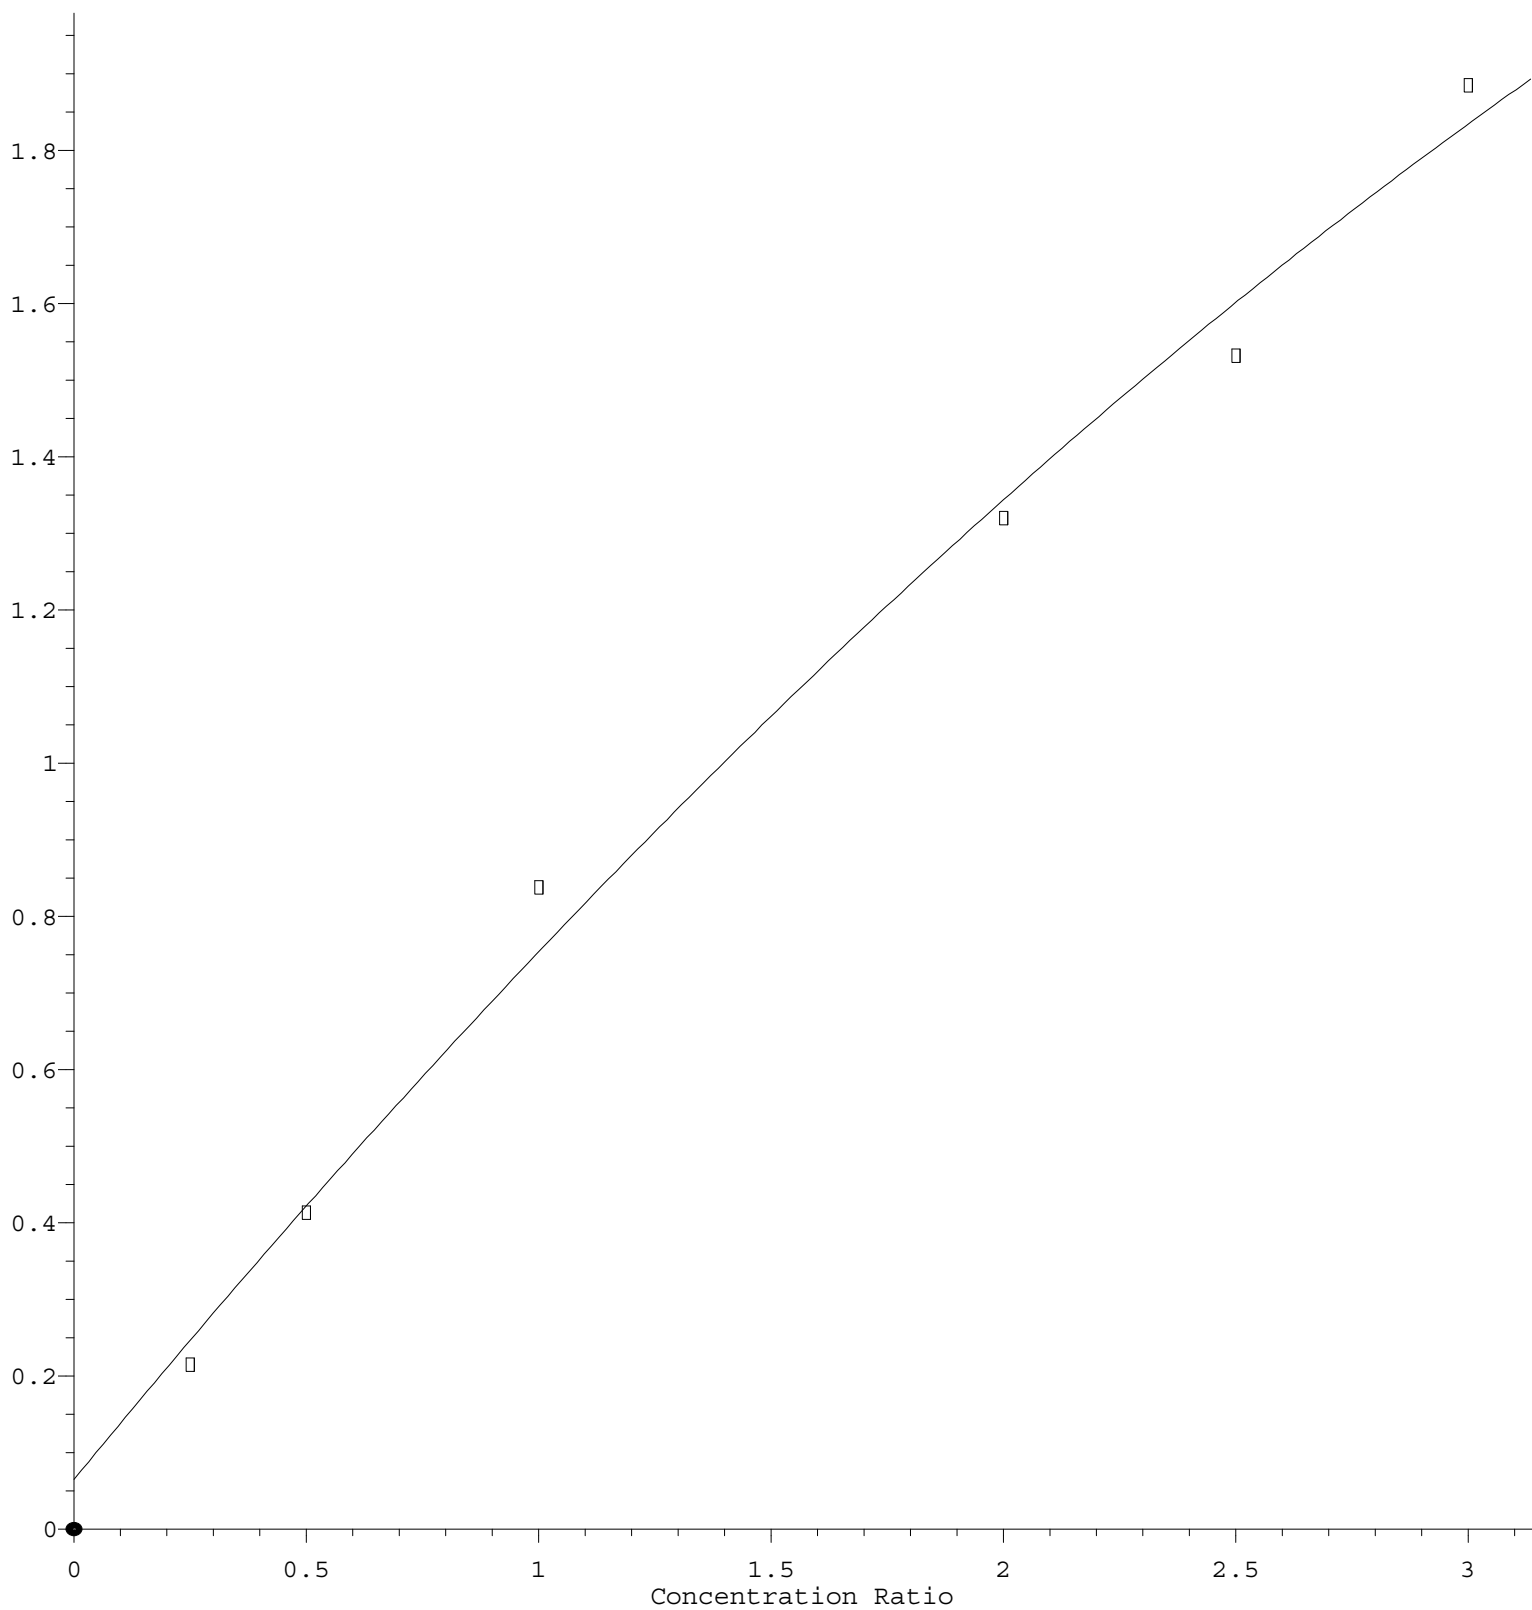

$R = -4.950e-002 A^2 + 7.384e-001 A + 6.500e-002$
Coef of Det (r^2) = 0.992514 Curve Fit: Quadratic
Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG071522.M
Calibration Table Last Updated: Fri Jul 15 15:54:11 2022

Phenanthrene

Response Ratio

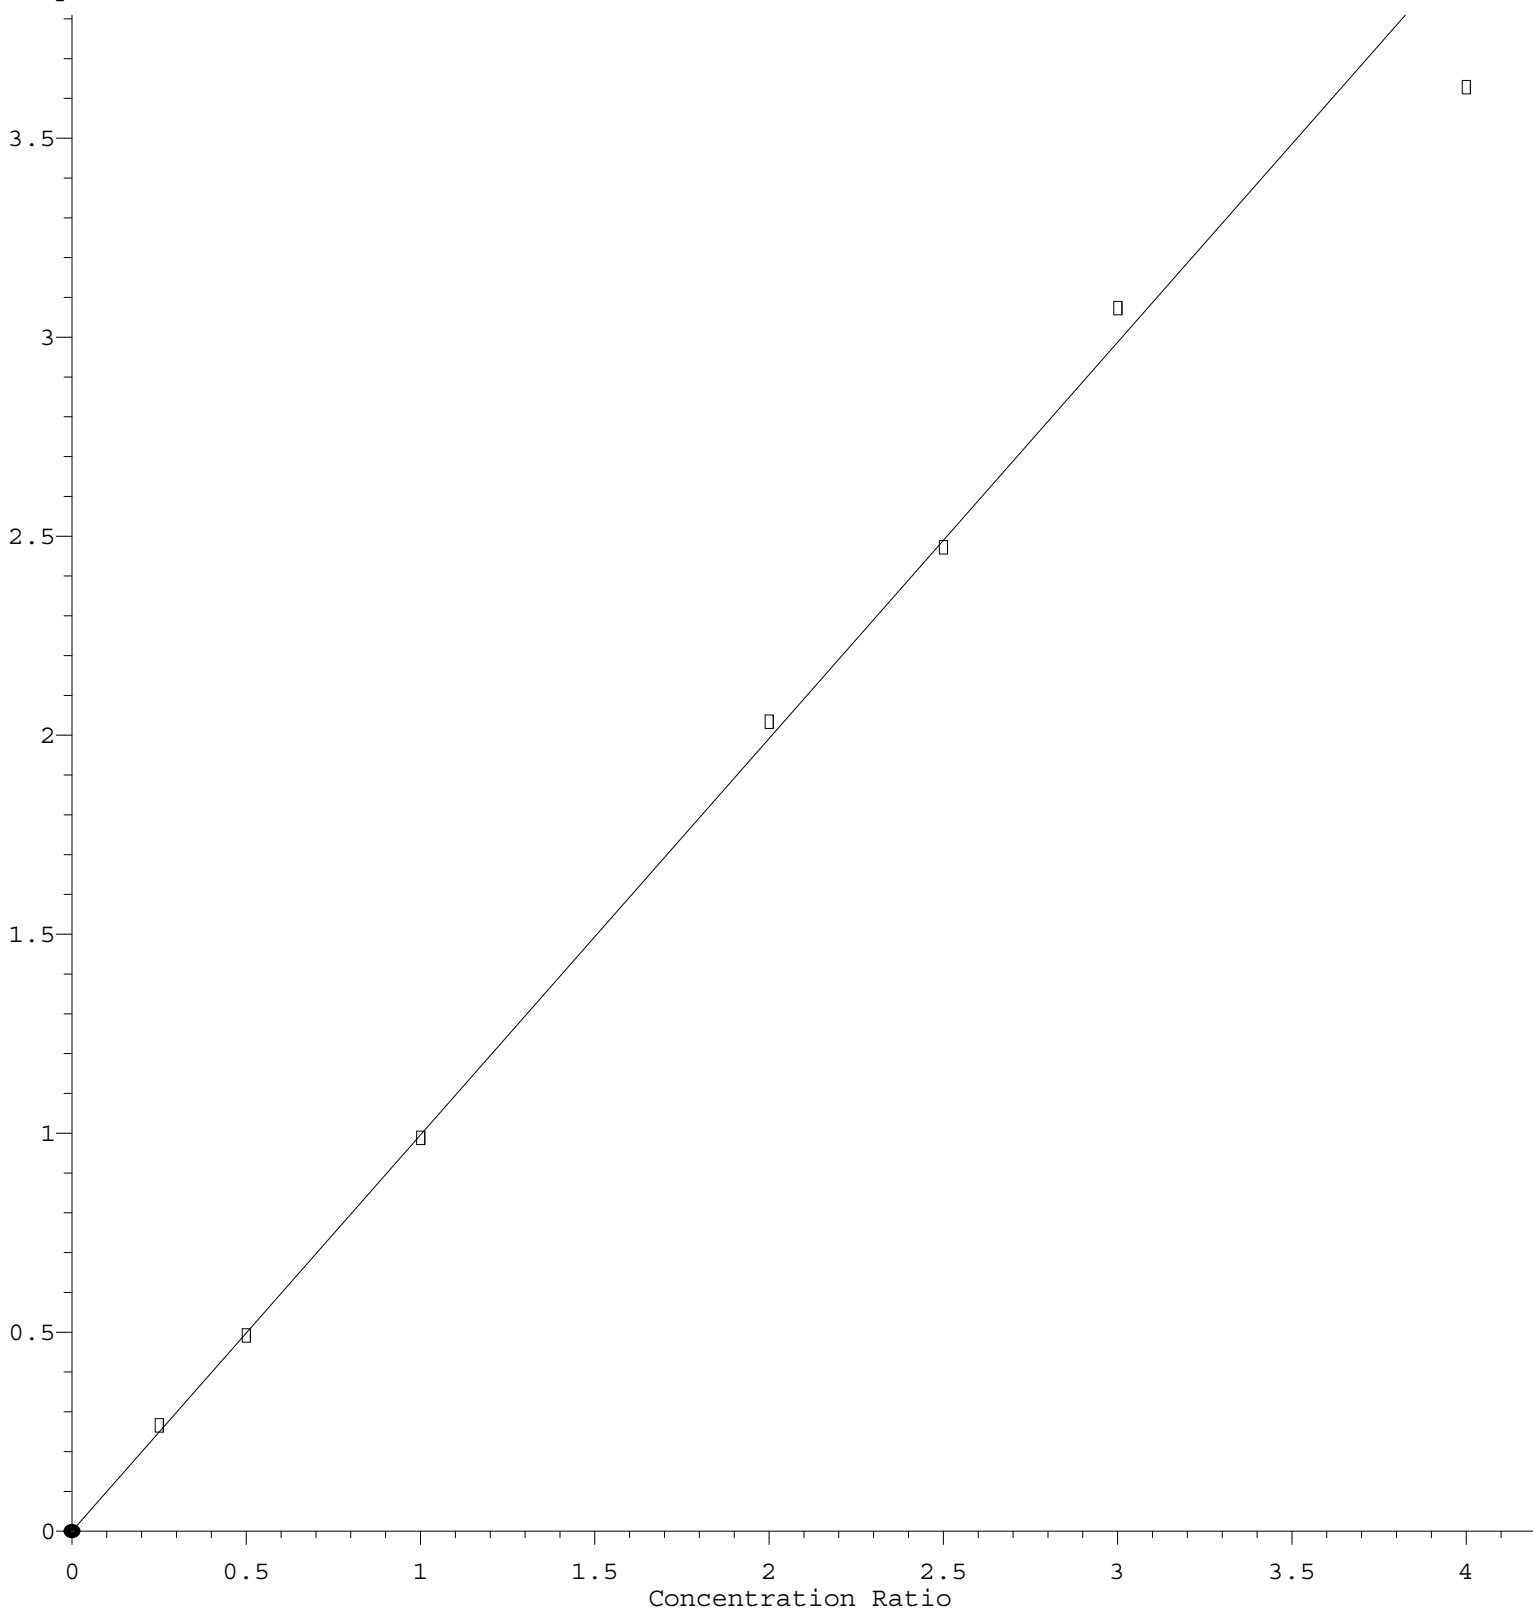


$$\text{Response} = 9.960\text{e-}001 * \text{Amt}$$

RF Rel Std Dev = 4.834% Curve Fit: Avg RF

Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG071522.M


Calibration Table Last Updated: Fri Jul 15 15:54:11 2022

2,4-Dinitrophenol

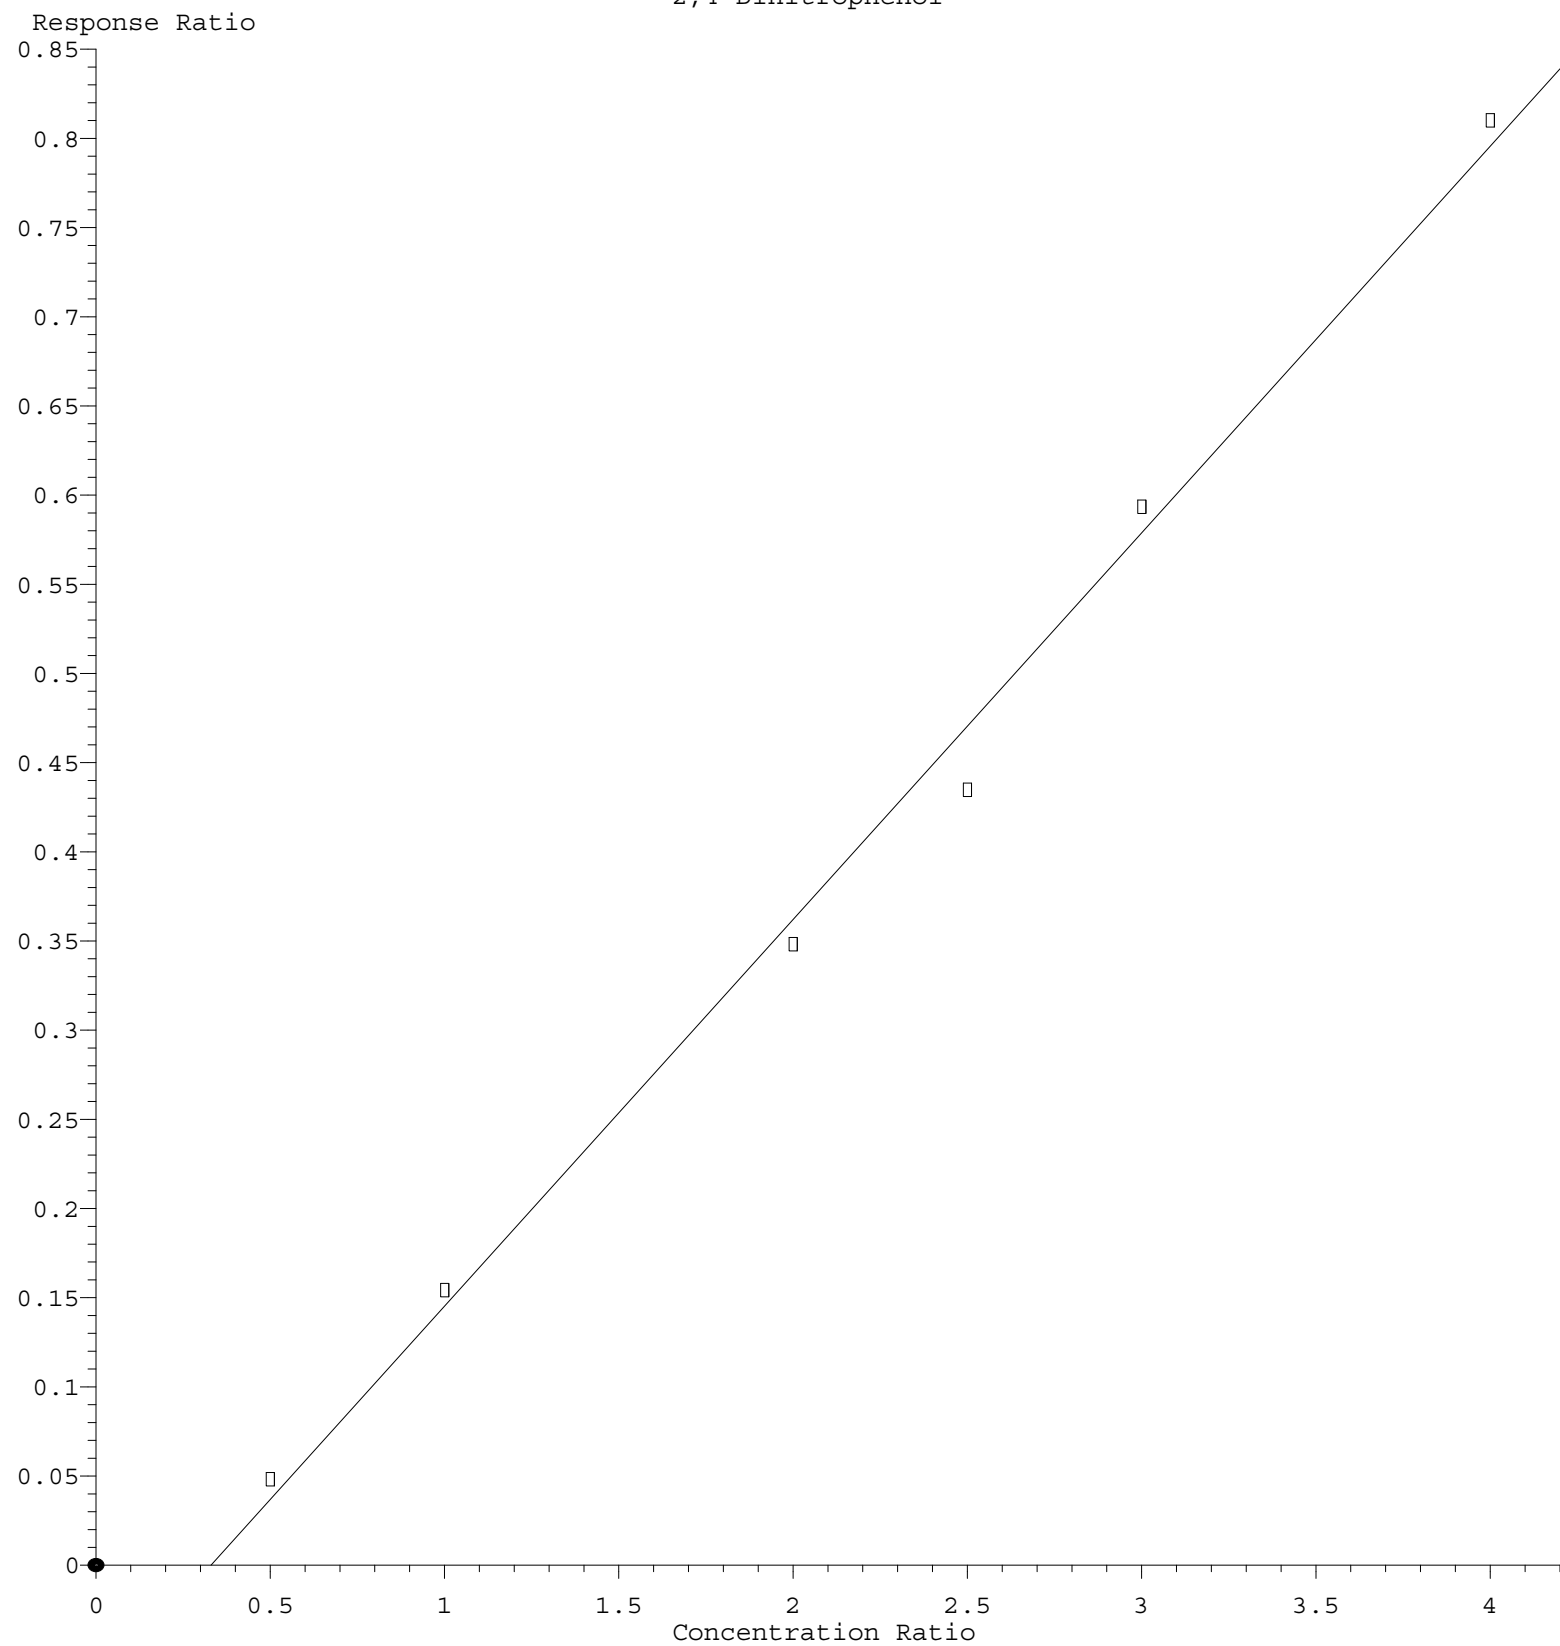


Response = 2.168e-001 * Amt - 7.151e-002
 Coef of Det (r^2) = 0.994669 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG071522.M
 Calibration Table Last Updated: Fri Jul 15 15:54:11 2022

Hexachlorocyclopentadiene

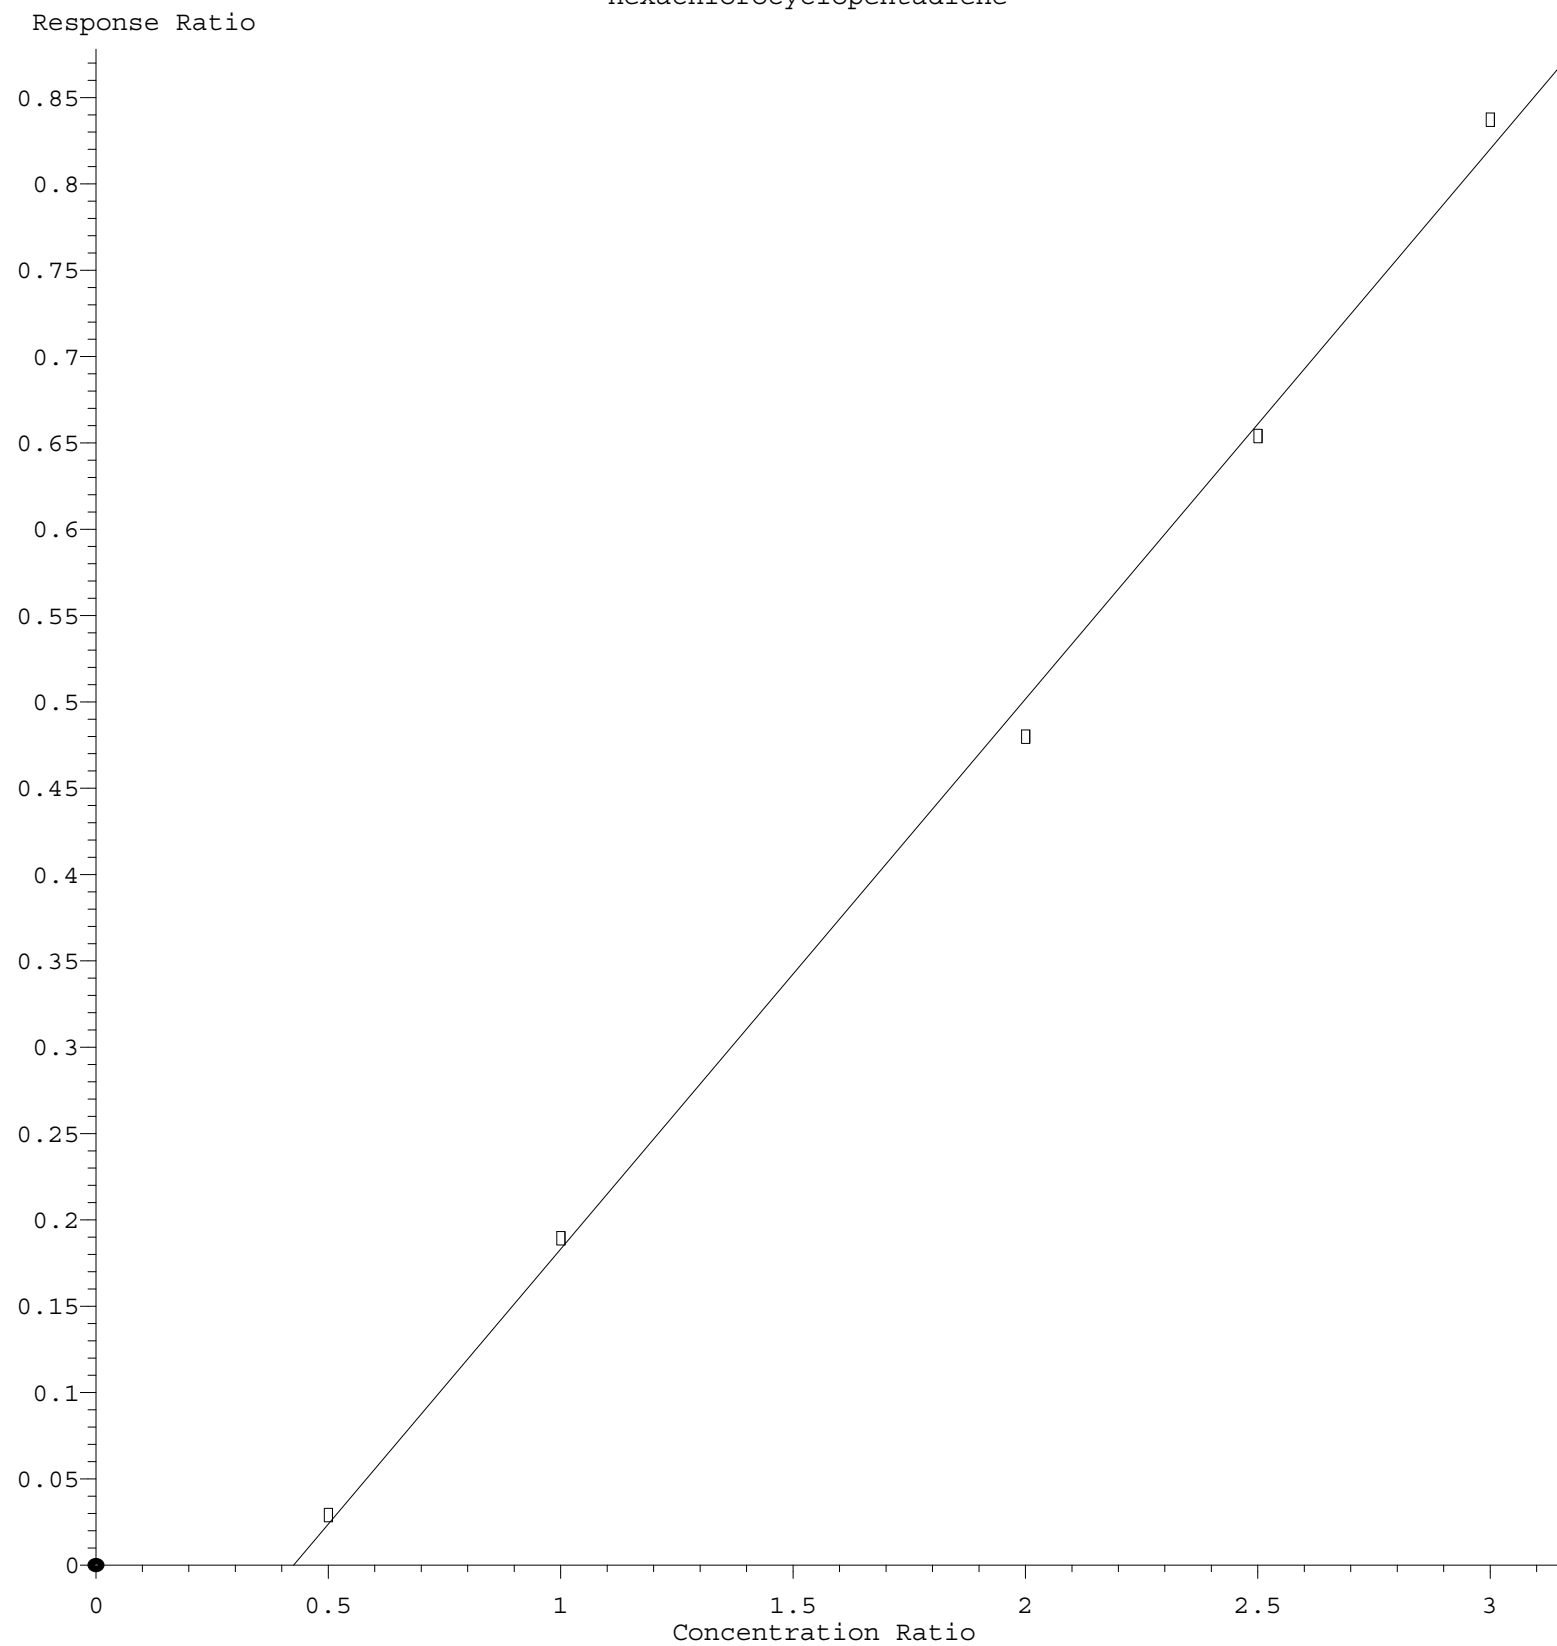

Response = $3.184 \times 10^{-1} \times \text{Amt} - 1.353 \times 10^{-1}$
Coef of Det (r^2) = 0.997991 Curve Fit: Linear
Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG071522.M
Calibration Table Last Updated: Fri Jul 15 15:54:11 2022

Benzoic acid

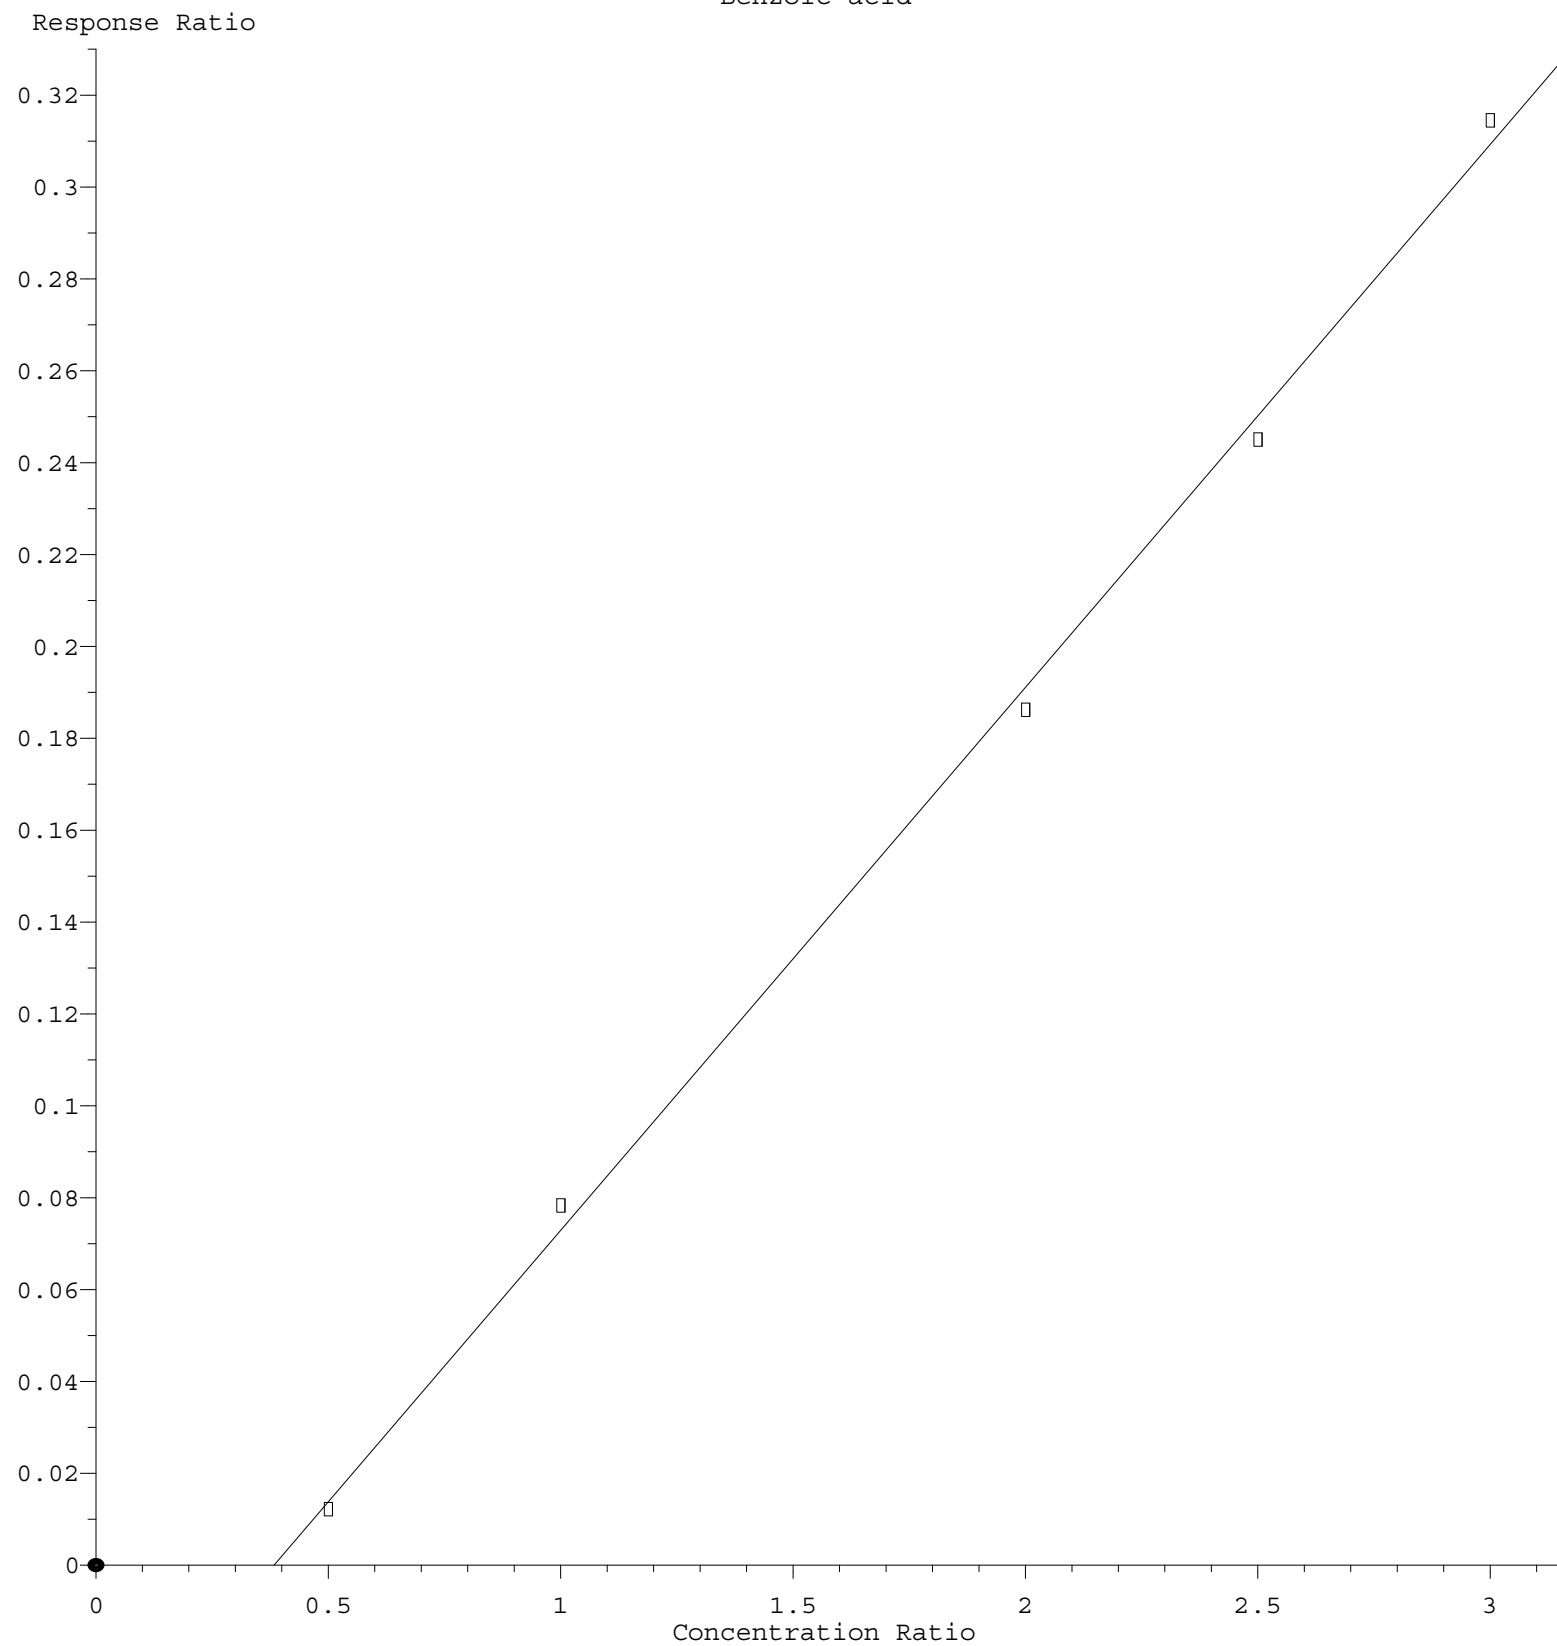

Response = $1.181e-001 * Amt - 4.527e-002$
 Coef of Det (r^2) = 0.998184 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG071522.M
 Calibration Table Last Updated: Fri Jul 15 15:54:11 2022