
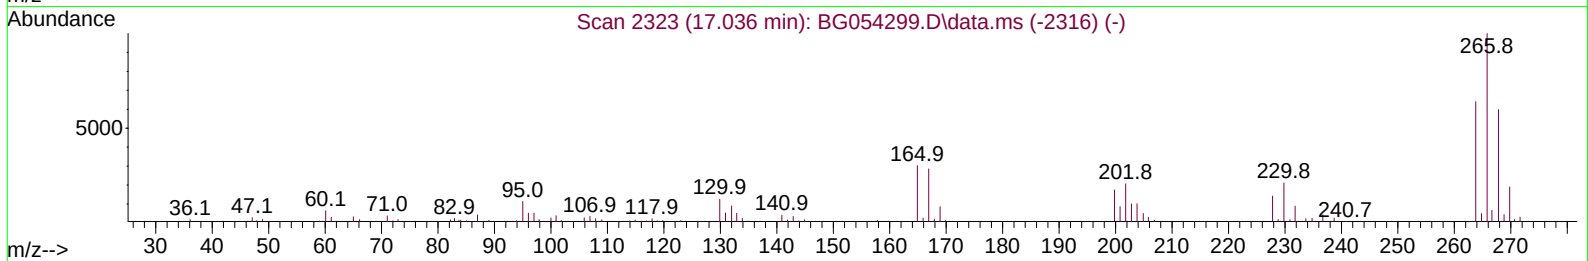
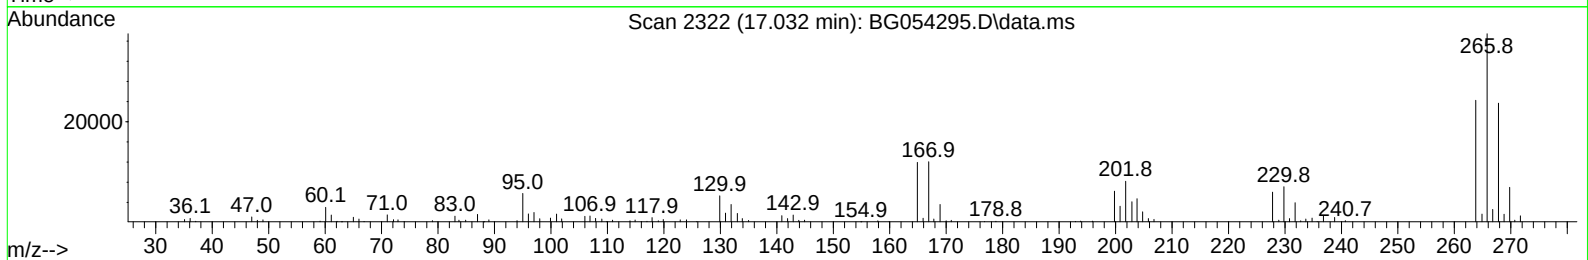


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071522\
Data File : BG054295.D
Acq On : 15 Jul 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 14:18:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 14:17:51 2022
Response via : Initial Calibration

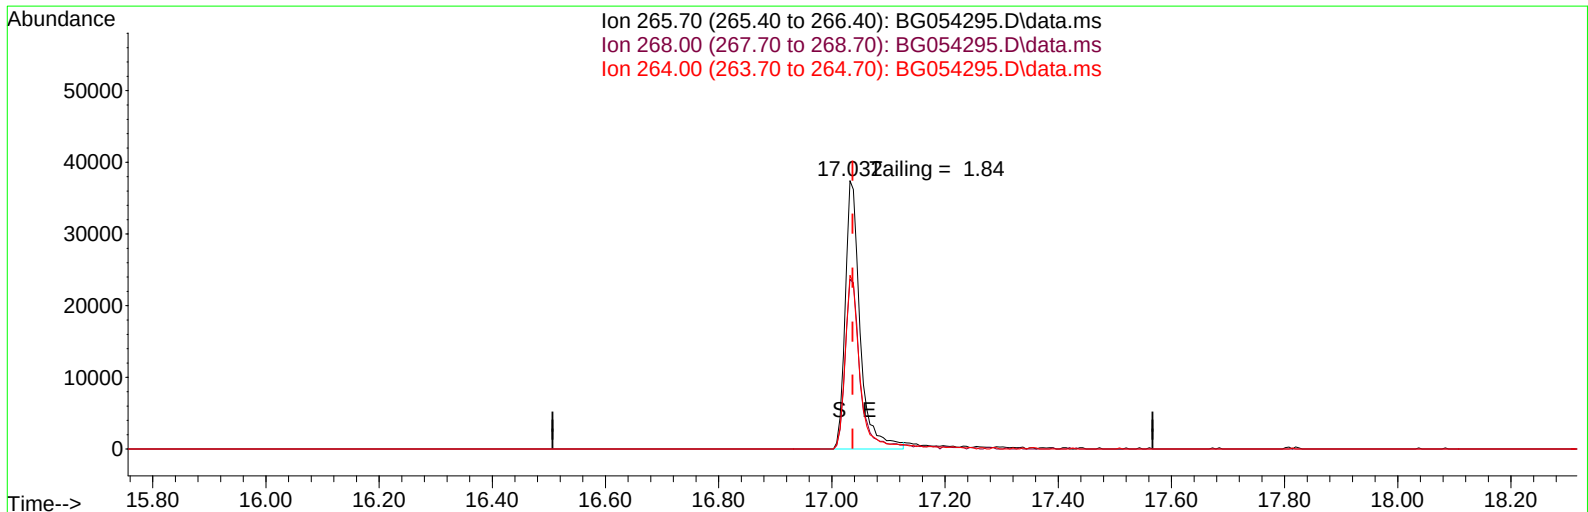

TIC: BG054295.D\data.ms

(70) Pentachlorophenol (C)




17.032min (-0.004) 25013.06 ng

response 70825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.19
264.00	66.20	64.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071522\
Data File : BG054295.D
Acq On : 15 Jul 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 14:18:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 14:17:51 2022
Response via : Initial Calibration

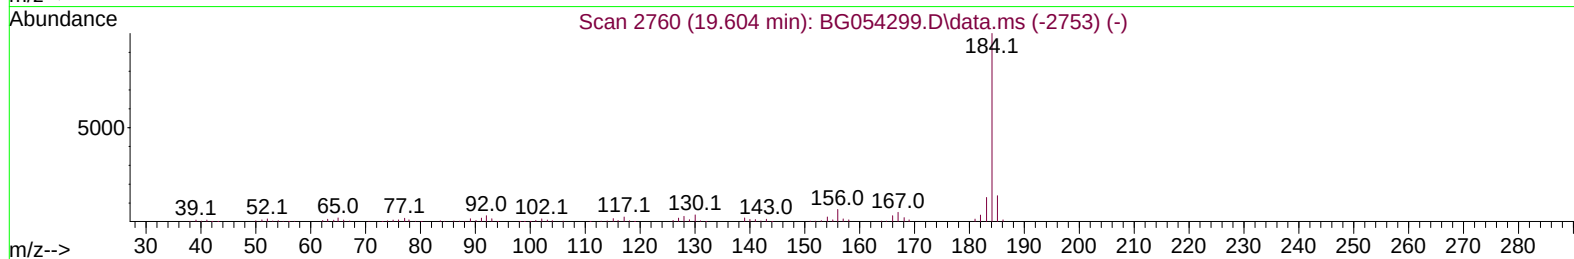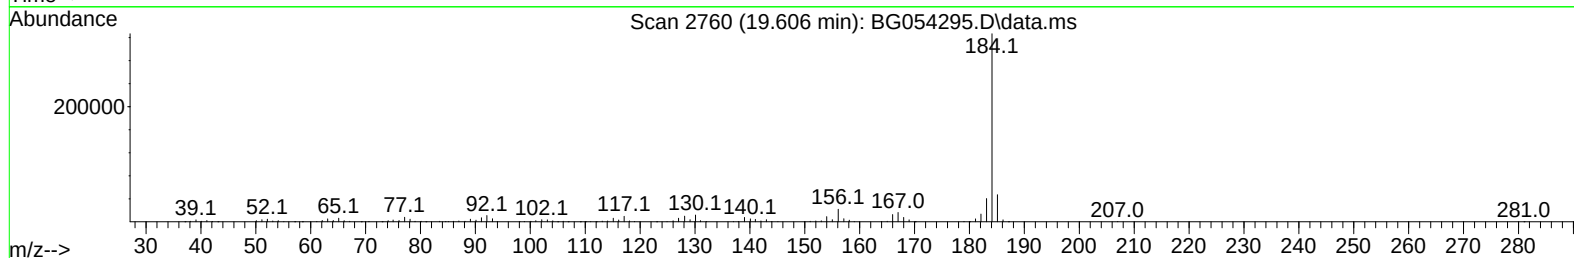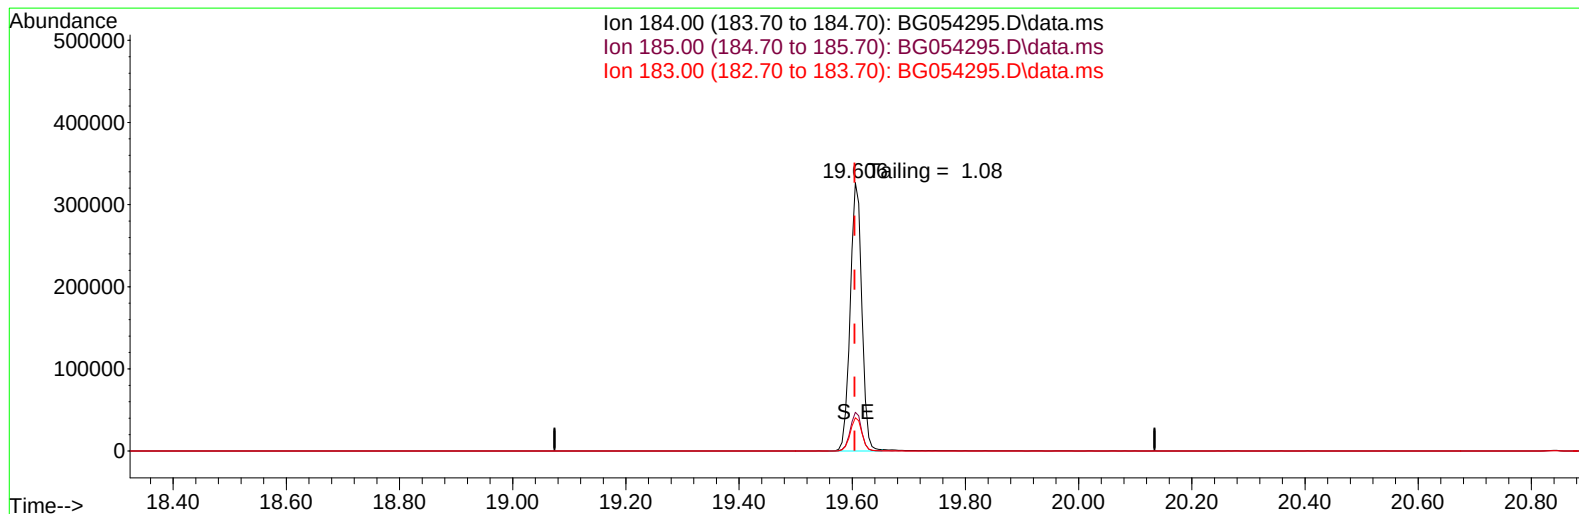

TIC: BG054295.D\data.ms

(77) Benzidine

19.606min (+ 0.002) 0.00 ng

response 466788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.47
183.00	11.10	12.42
0.00	0.00	0.00