
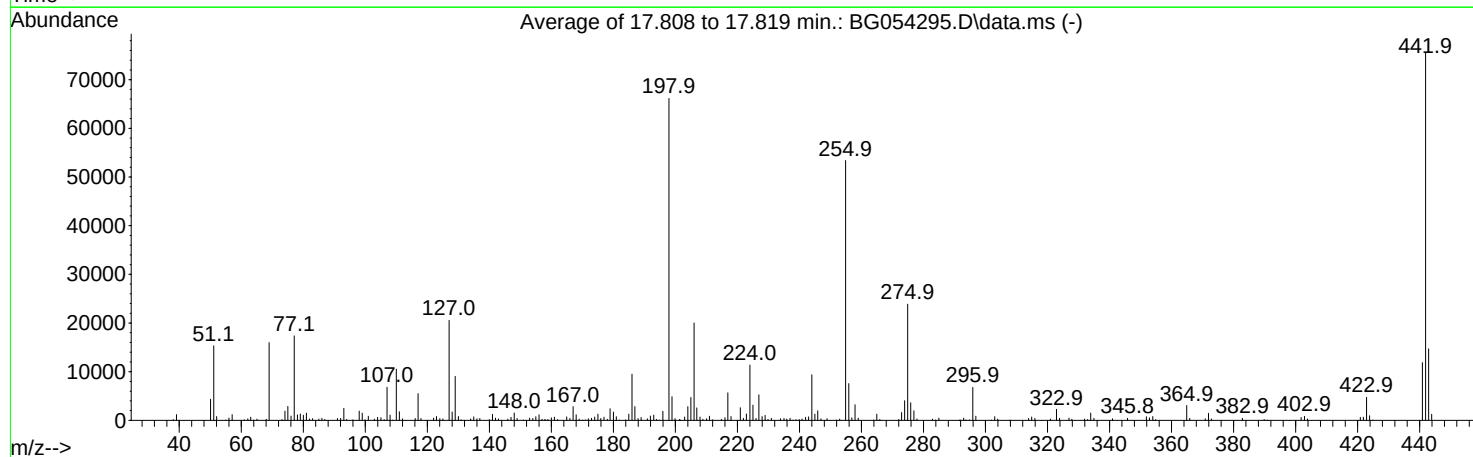


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071522\
 Data File : BG054295.D
 Acq On : 15 Jul 2022 9:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

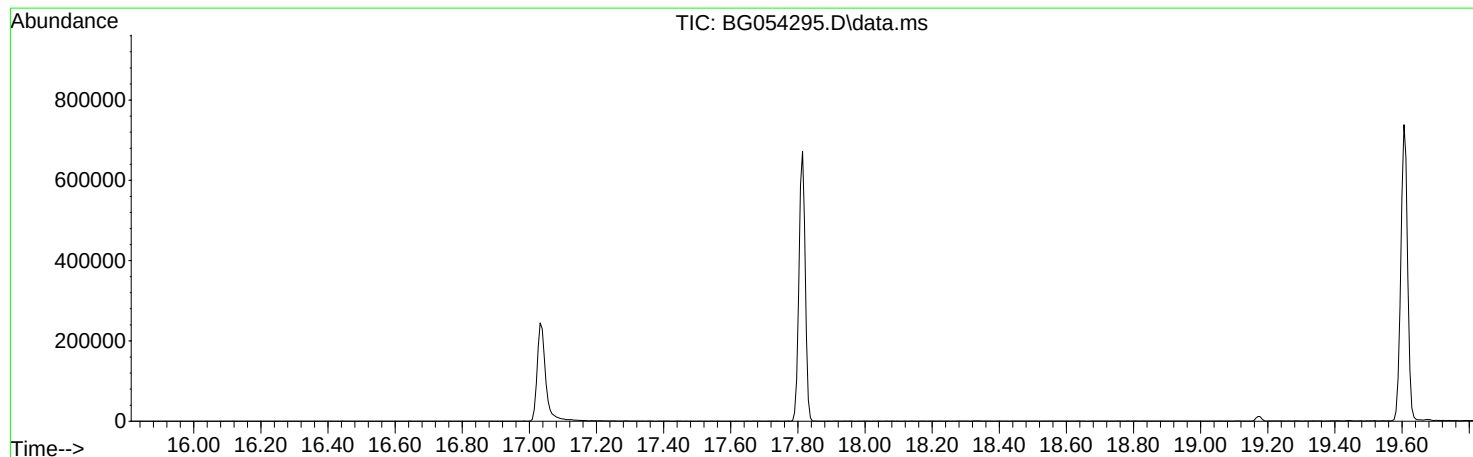




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	15335	PASS
68	69	0.00	2	1.5	233	PASS
69	198	0.00	100	24.1	15973	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.1	20557	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66149	PASS
199	198	5	9	7.4	4872	PASS
275	198	10	60	36.1	23859	PASS
365	198	1	100	4.6	3059	PASS
441	198	0.01	100	18.0	11886	PASS
442	442	50	100	100.0	75576	PASS
443	442	15	24	19.4	14699	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071522\
Data File : BG054295.D
Acq On : 15 Jul 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 15 14:18:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 14:17:51 2022
Response via : Initial Calibration

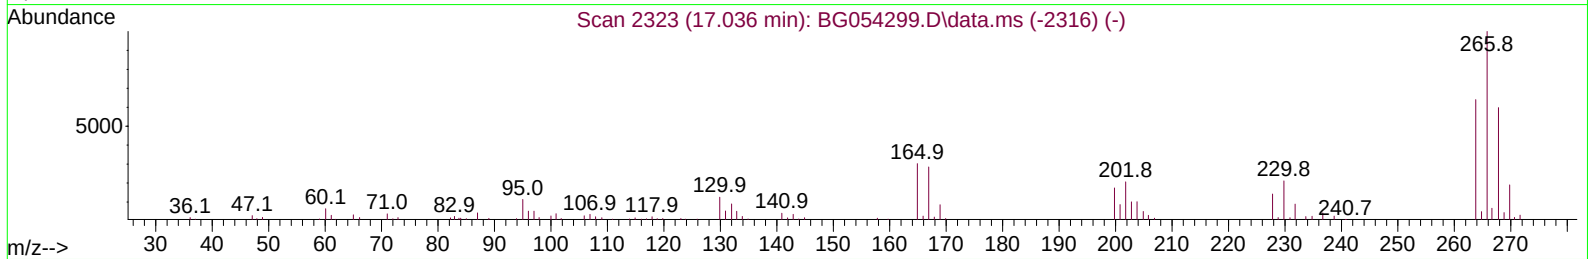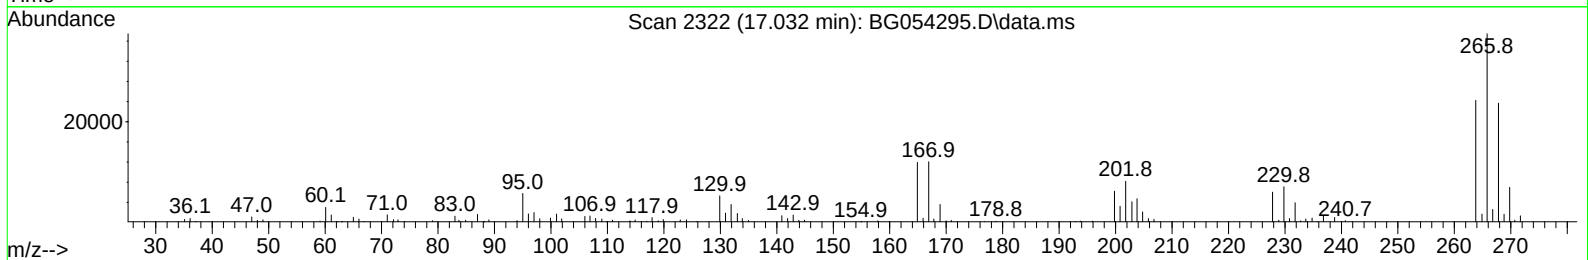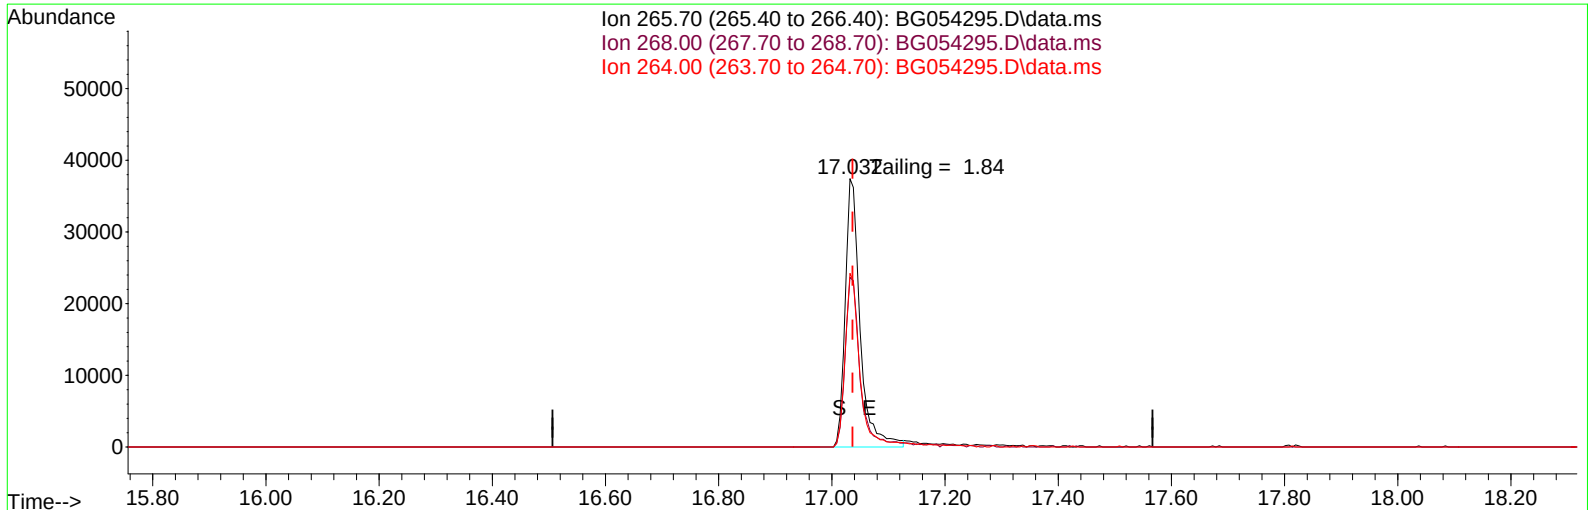

TIC: BG054295.D\data.ms

(70) Pentachlorophenol (C)

17.032min (-0.004) 25013.06 ng




response 70825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.19
264.00	66.20	64.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071522\
Data File : BG054295.D
Acq On : 15 Jul 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 15 14:18:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 14:17:51 2022
Response via : Initial Calibration

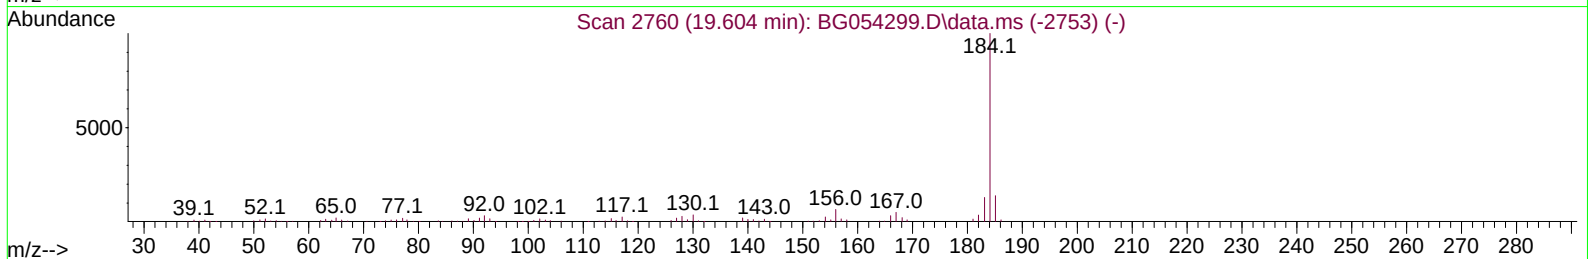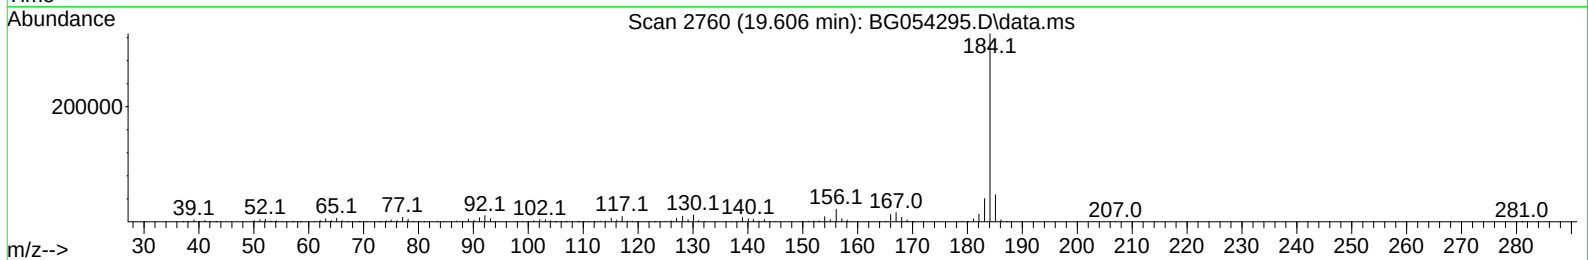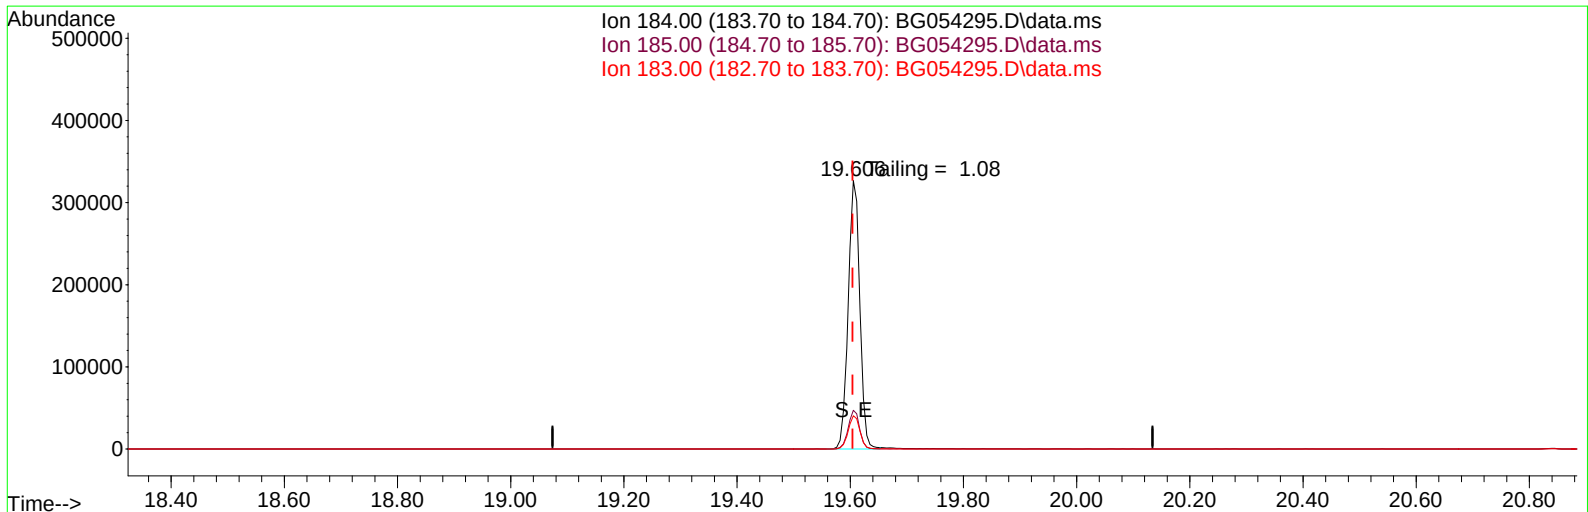

TIC: BG054295.D\data.ms

(77) Benzidine

19.606min (+ 0.002) 0.00 ng

response 466788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.47
183.00	11.10	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_G	<u>BG054295.D</u>
Compound Name	Response	Retention Time
DDT	273881	20.83
DDD	819	20.39
DDE	53	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
872	274753	0.32

Instrument :
BNA_G
ClientSampleId :
DFTPP