
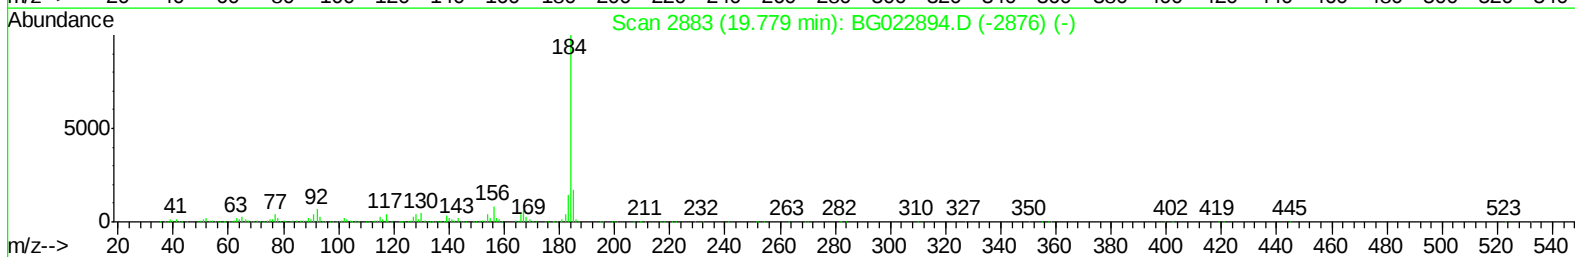
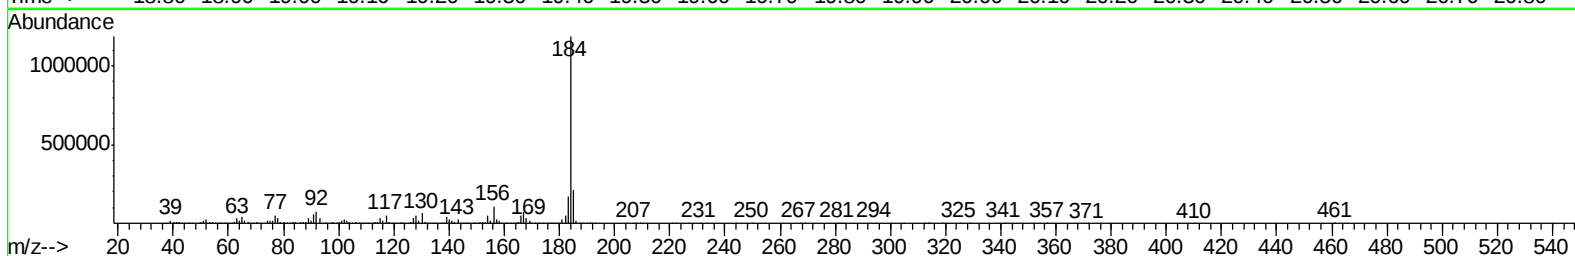


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071616\
Data File : BG023138.D
Acq On : 16 Jul 2016 8:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 15:58:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

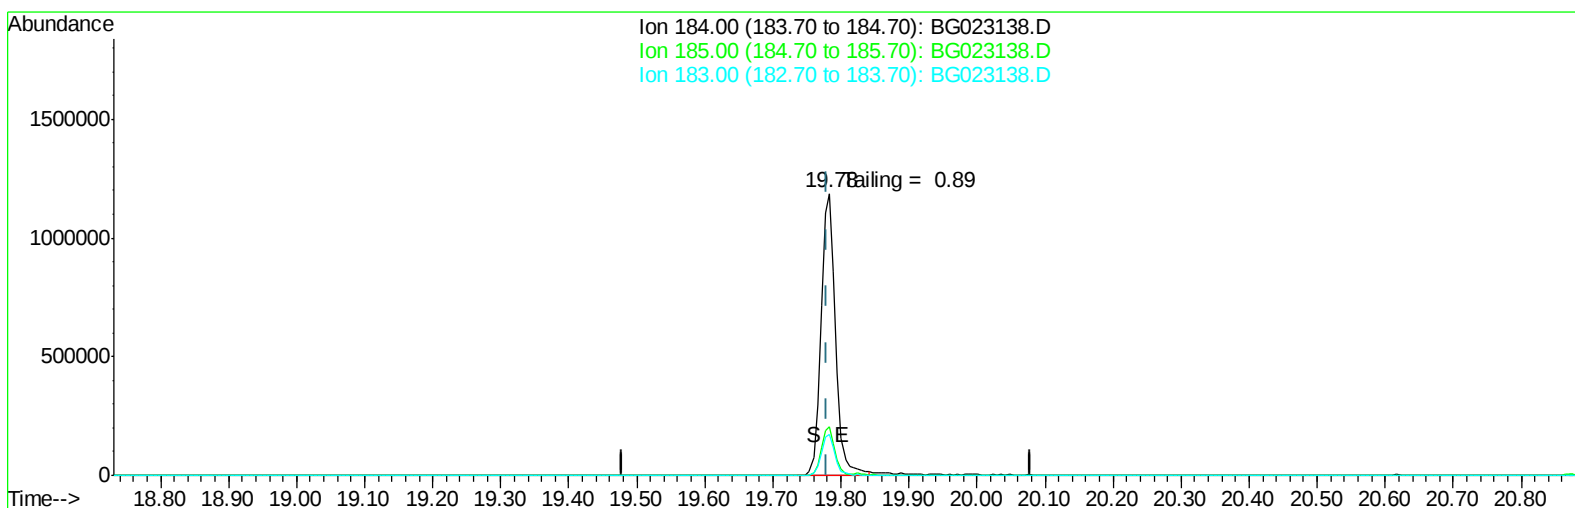

TIC: BG023138.D

(76) Benzidine




19.783min (+0.004) 19317.13ng

response 1810910

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	17.51
183.00	13.40	14.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071616\
Data File : BG023138.D
Acq On : 16 Jul 2016 8:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 15:58:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

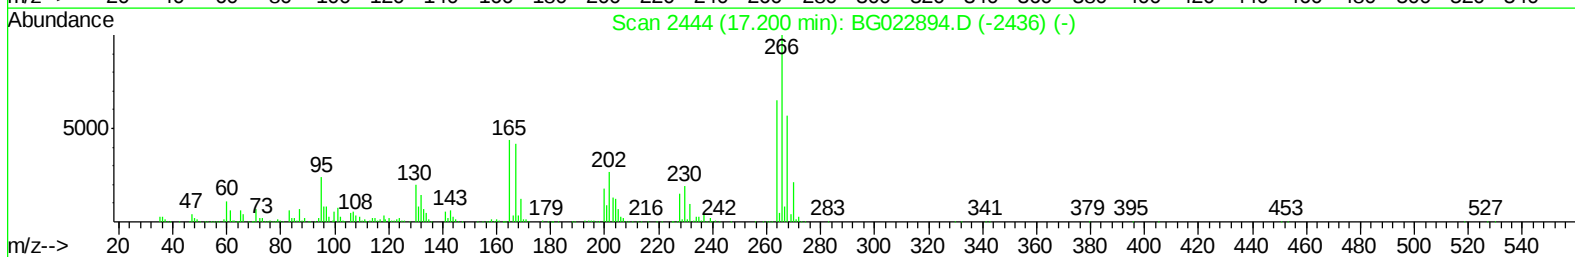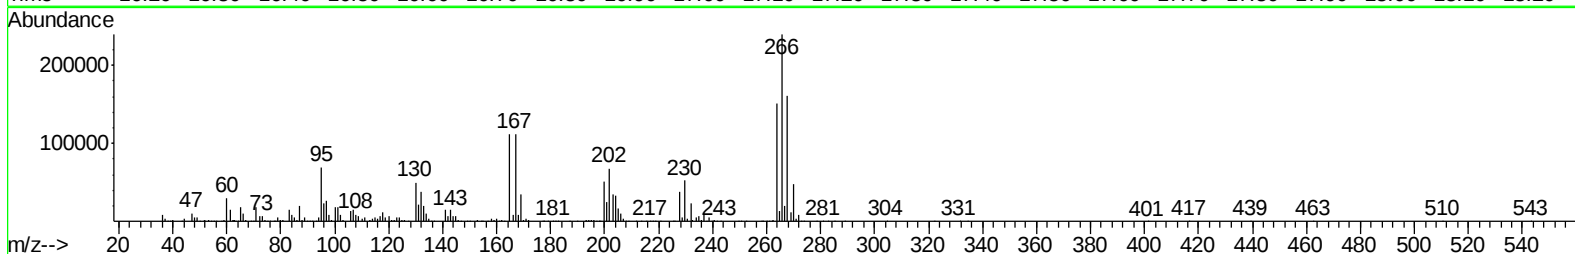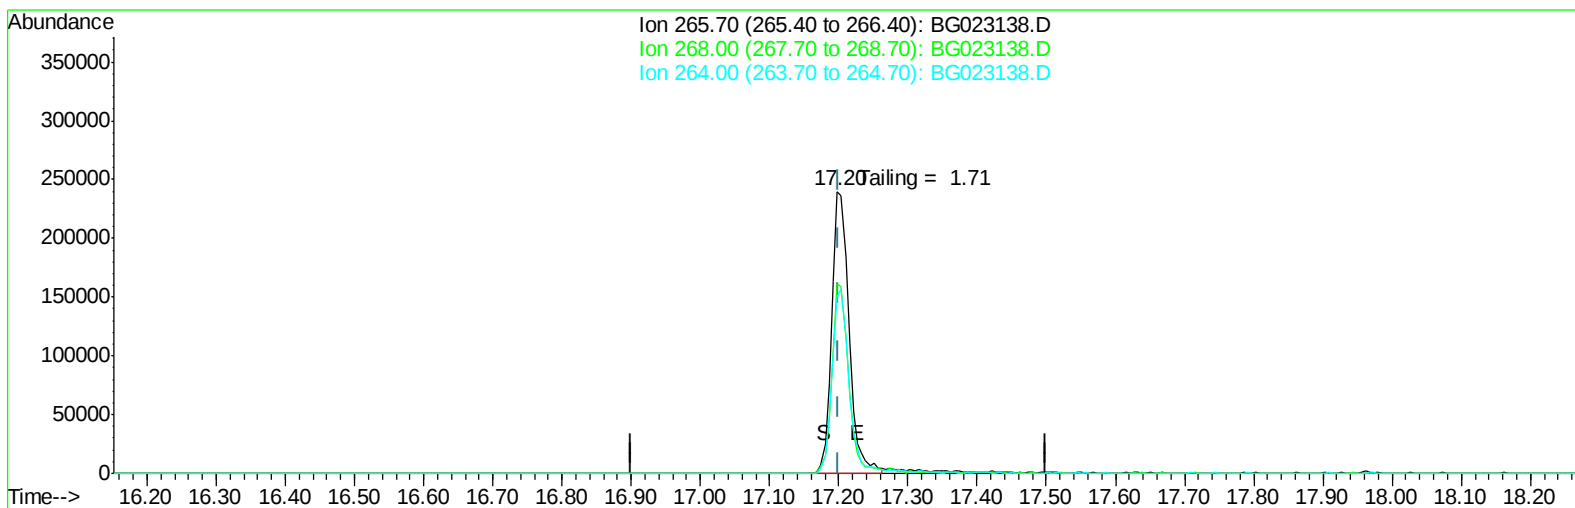

TIC: BG023138.D

(69) Pentachlorophenol (C)

17.198min (-0.002) 46291.36ng

response 415167

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.09
264.00	63.20	62.78
0.00	0.00	0.00