

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071616\
 Data File : BG023142.D
 Acq On : 16 Jul 2016 11:38
 Operator : UM/SJ
 Sample : H4015-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C5-21

Quant Time: Jul 18 01:19:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 12 18:30:58 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	95190	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	439948	20.00	ng	0.00
38) Acenaphthene-d10	14.80	164	334814	20.00	ng	0.00
63) Phenanthrene-d10	17.55	188	835321	20.00	ng	0.00
75) Chrysene-d12	21.85	240	917772	20.00	ng	0.00
86) Perylene-d12	25.22	264	913818	20.00	ng	0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	699330	120.16	ng	0.00
7) Phenol-d6	7.30	99	1109936	121.76	ng	0.00
23) Nitrobenzene-d5	9.32	82	788181	76.71	ng	0.00
41) 2,4,6-Tribromophenol	16.29	330	579225	96.26	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	1564502	73.60	ng	0.00
78) Terphenyl-d14	20.15	244	2403662	81.94	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.24	163	456241	16.68	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071616\
Data File : BG023142.D
Acq On : 16 Jul 2016 11:38
Operator : UM/SJ
Sample : H4015-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C5-21

Quant Time: Jul 18 01:19:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

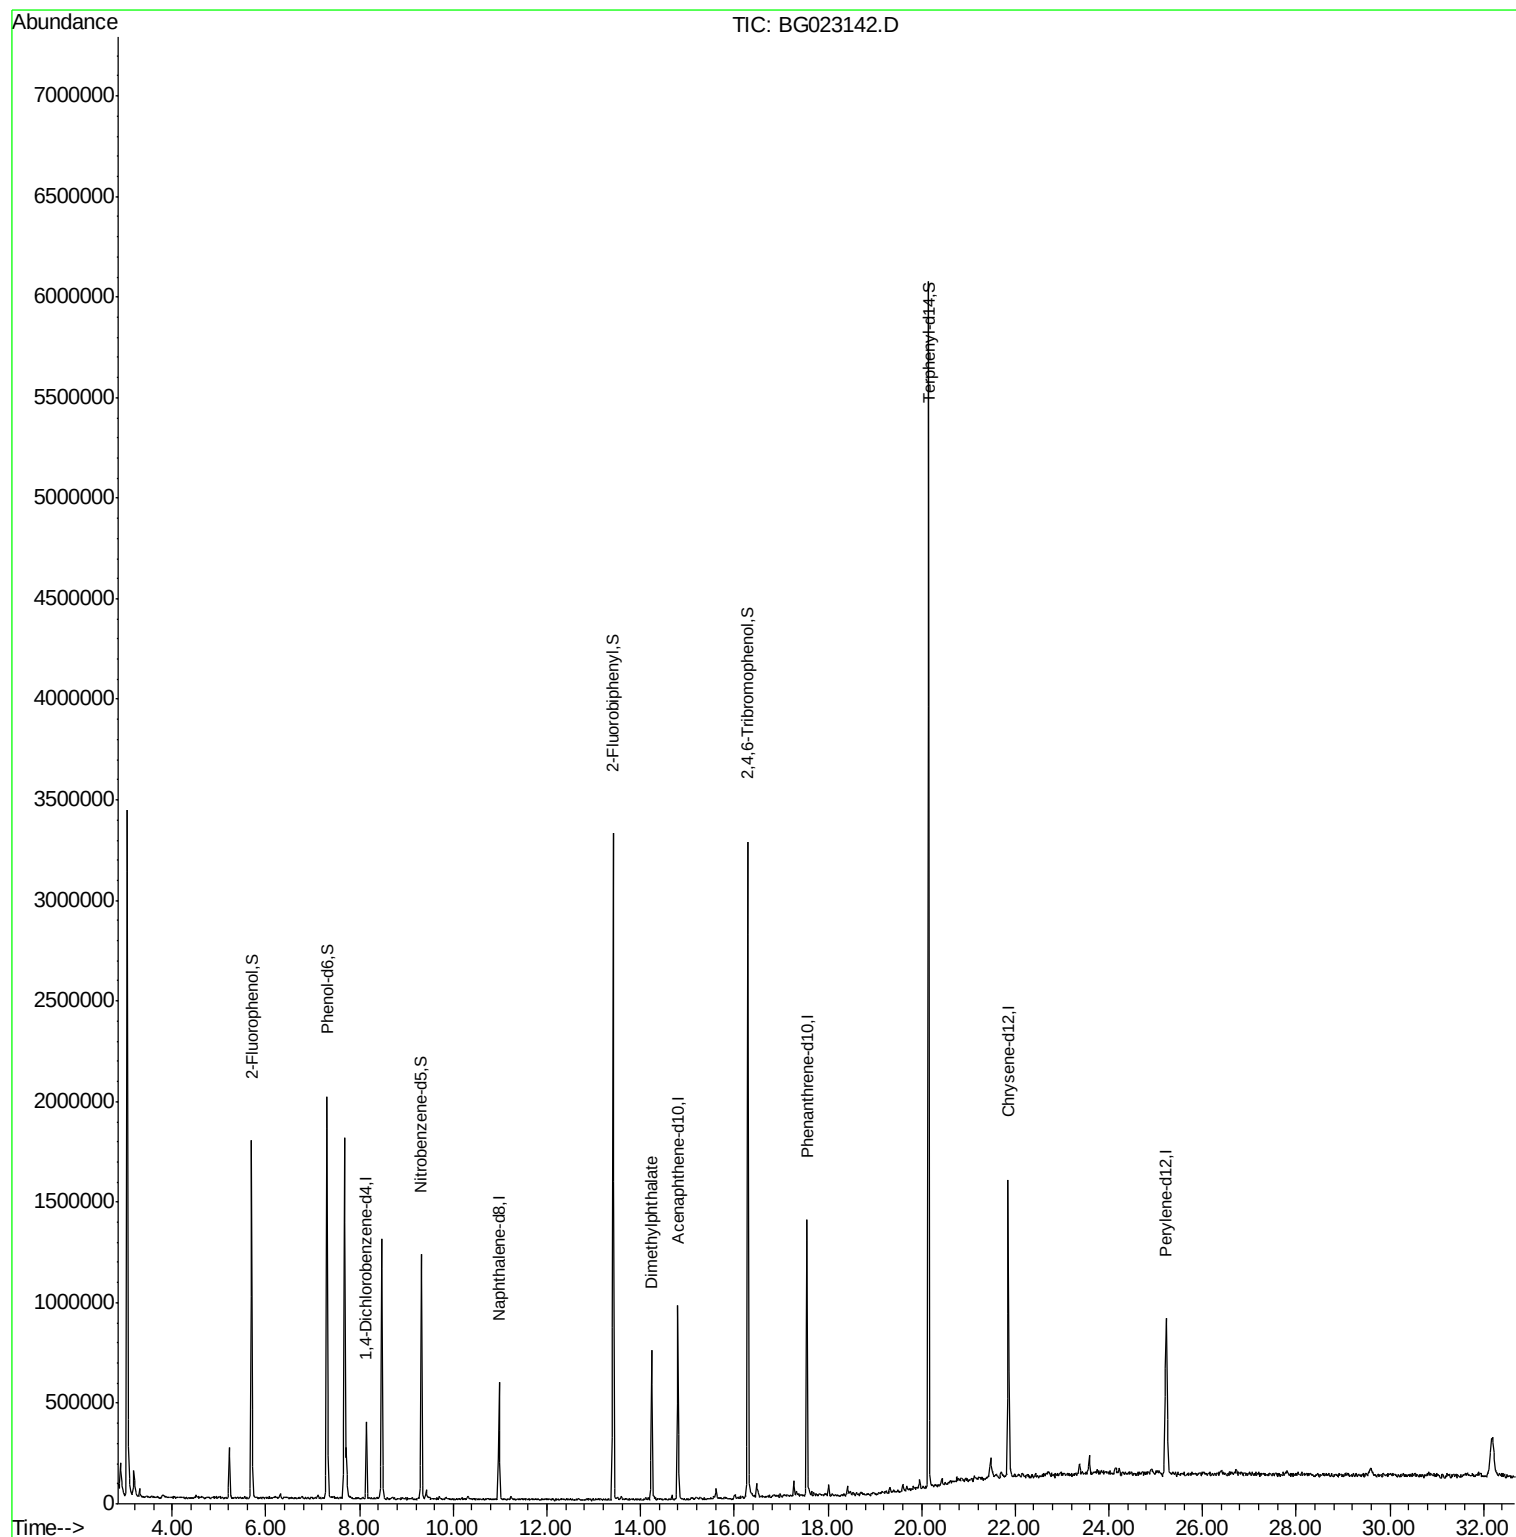




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.14 min Scan# 903
Delta R.T. -0.01 min
Lab File: BG023142.D
Acq: 16 Jul 2016 11:38

Instrument :
BNA_G
ClientSampleId :
C5-21

Tgt Ion:152 Resp: 95190
Ion Ratio Lower Upper
152 100
150 157.8 144.7 217.1
115 72.1 64.0 96.0

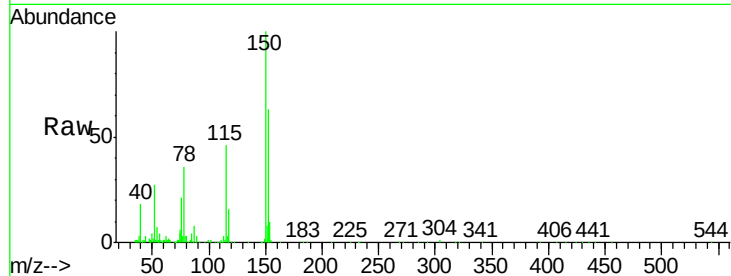


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

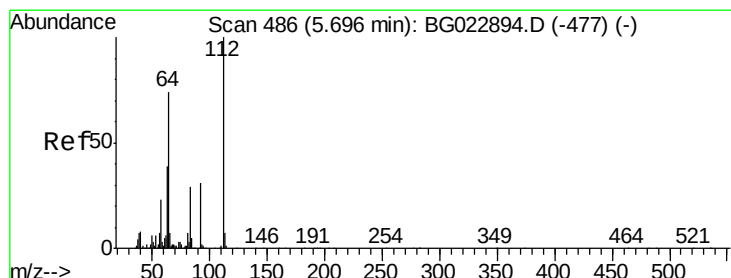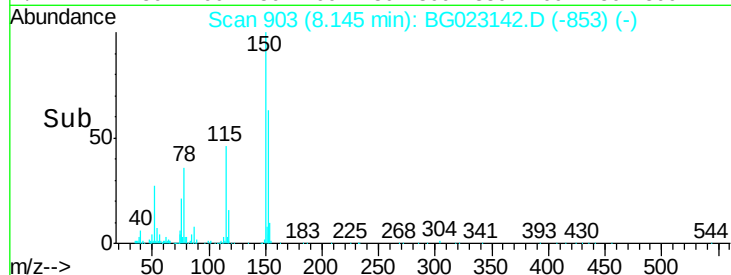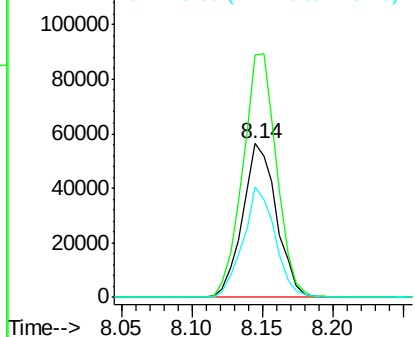



#5


2-Fluorophenol
Concen: 120.16 ng
RT: 5.69 min Scan# 486
Delta R.T. -0.00 min
Lab File: BG023142.D
Acq: 16 Jul 2016 11:38

Tgt Ion:112 Resp: 699330
Ion Ratio Lower Upper
112 100
64 70.4 59.0 88.4
63 40.2 37.8 56.8

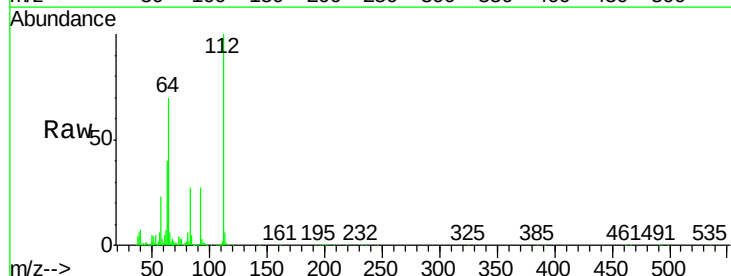

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

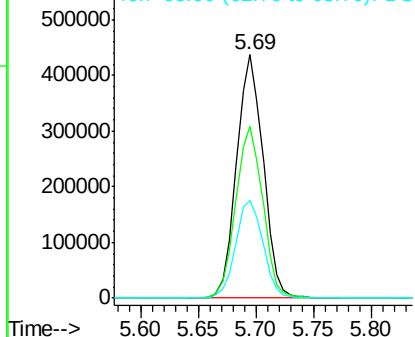



#7

Phenol-d6

Concen: 121.76 ng

RT: 7.30 min Scan# 760

Delta R.T. -0.00 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38

Instrument :

BNA_G

ClientSampleId :

C5-21


Tgt Ion: 99 Resp: 1109936

Ion Ratio Lower Upper




99 100

42 20.2 17.8 26.6

71 48.9 41.5 62.3

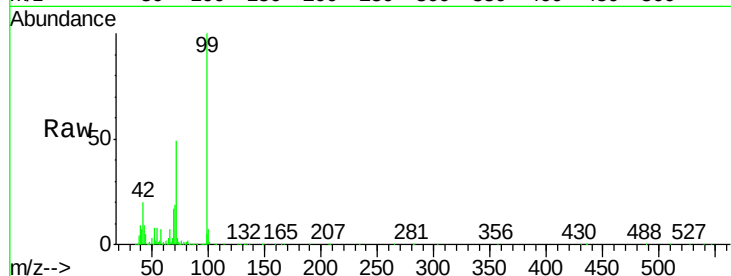

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

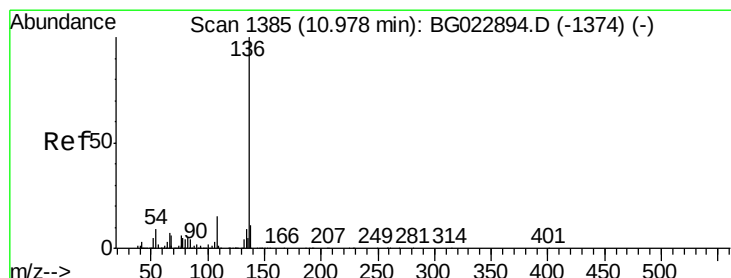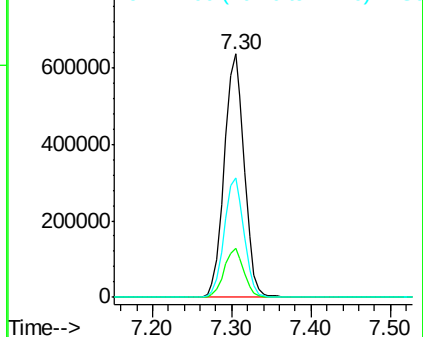

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.98 min Scan# 1385

Delta R.T. -0.00 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38

Tgt Ion: 136 Resp: 439948


Ion Ratio Lower Upper

136 100



137 10.6 9.6 14.4


54 8.3 7.3 10.9

68 6.9 5.3 7.9

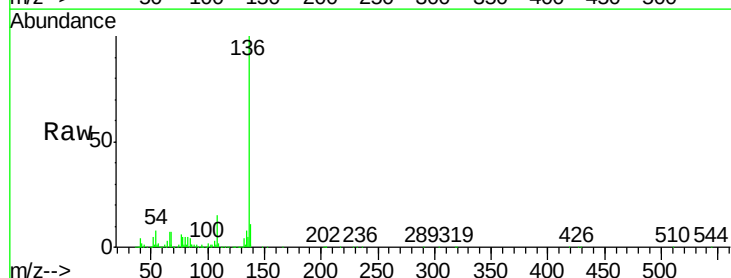

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




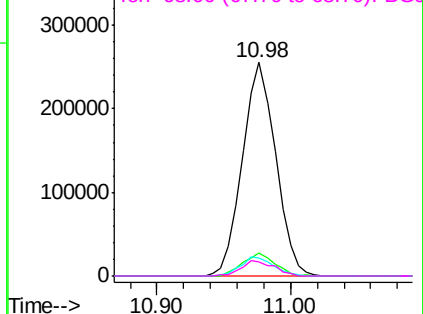


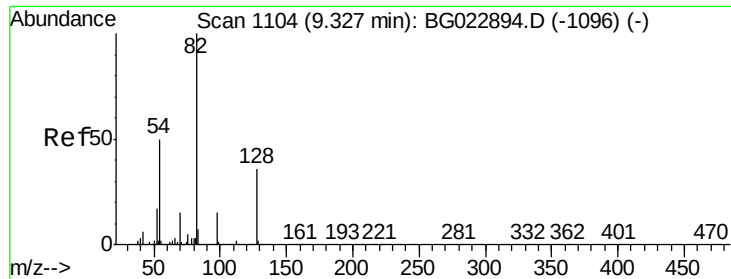

#23
 Nitrobenzene-d5
 Concen: 76.71 ng
 RT: 9.32 min Scan# 1103
 Delta R.T. -0.01 min
 Lab File: BG023142.D
 Acq: 16 Jul 2016 11:38




Instrument :
 BNA_G
 ClientSampleID :
 C5-21


Tgt Ion	Ratio	Lower	Upper
82	100		
128	31.8	24.4	36.6
54	48.6	41.4	62.0

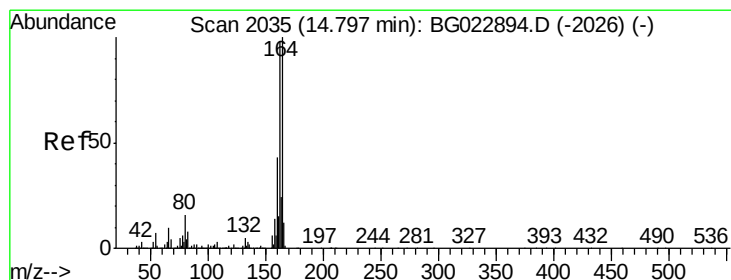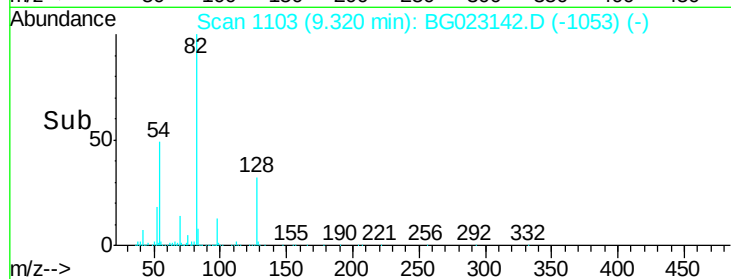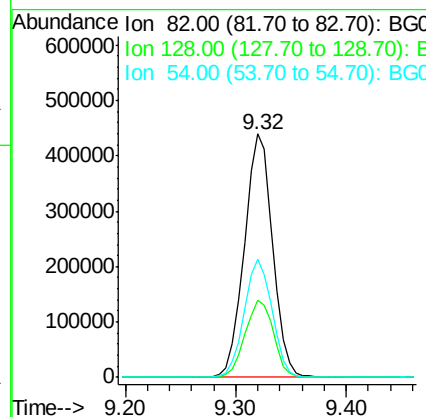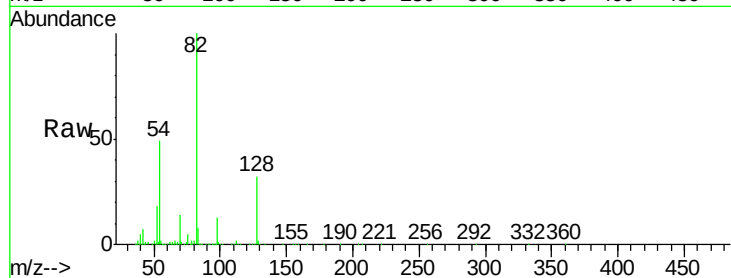

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.80 min Scan# 2035
 Delta R.T. -0.00 min
 Lab File: BG023142.D
 Acq: 16 Jul 2016 11:38

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.7	87.7	131.5
160	46.9	37.2	55.8

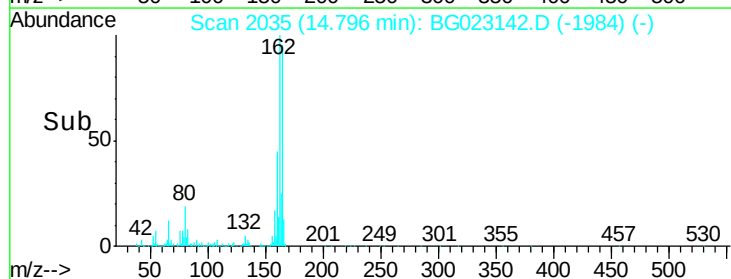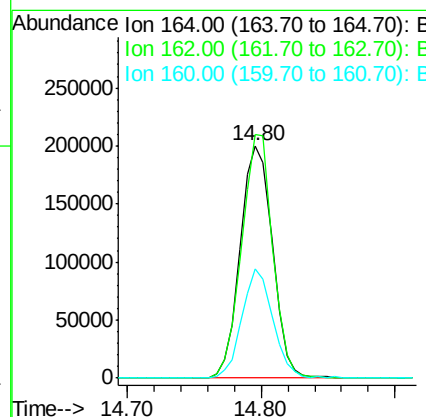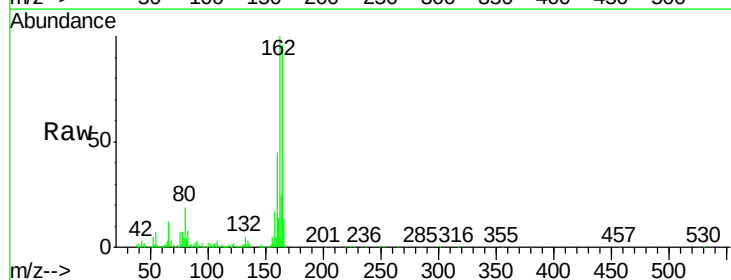


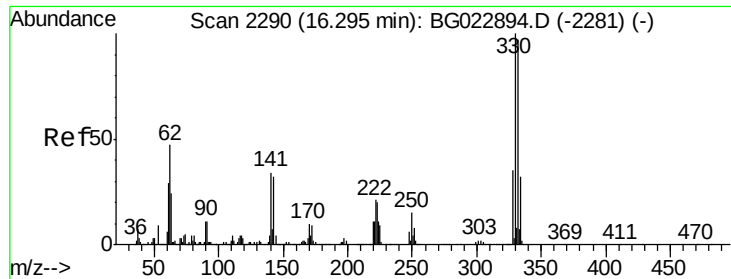




#41
 2,4,6-Tribromophenol
 Concen: 96.26 ng
 RT: 16.29 min Scan# 2289
 Delta R.T. -0.01 min
 Lab File: BG023142.D
 Acq: 16 Jul 2016 11:38

Instrument :
 BNA_G
 ClientSampled :
 C5-21

Tgt Ion	Ratio	Lower	Upper
330	100		
332	98.2	77.4	116.2
141	40.6	31.7	47.5

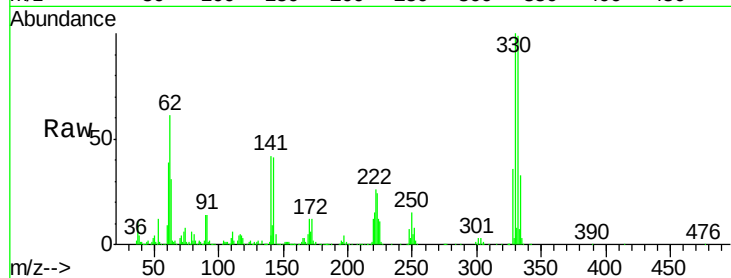


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

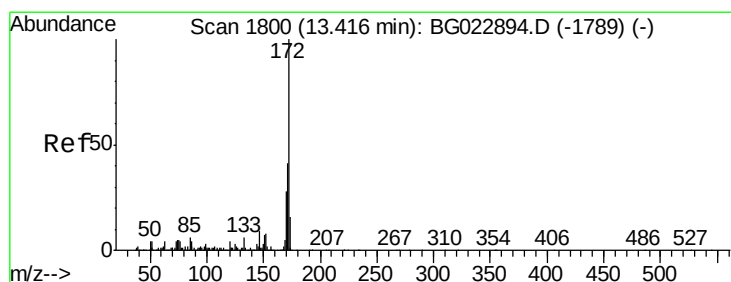
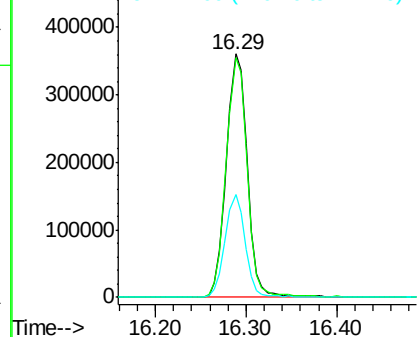



#44
 2-Fluorobiphenyl
 Concen: 73.60 ng
 RT: 13.42 min Scan# 1800
 Delta R.T. -0.00 min
 Lab File: BG023142.D
 Acq: 16 Jul 2016 11:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.3	31.6	47.4
170	26.7	21.3	31.9

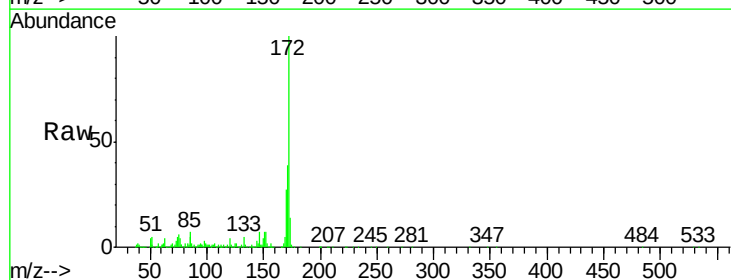

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

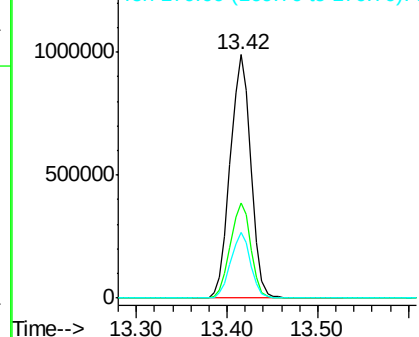

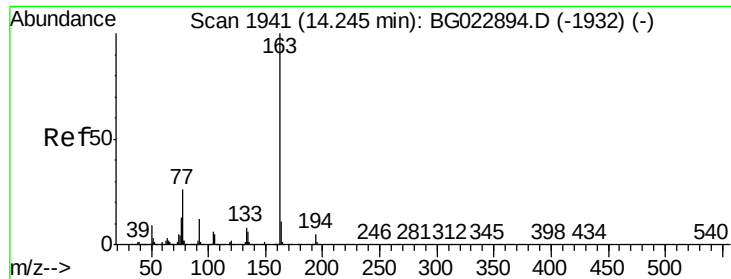

#49

Dimethylphthalate

Concen: 16.68 ng

RT: 14.24 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38

Instrument :

BNA_G

ClientSampleId :

C5-21


Tgt Ion:163 Resp: 456241

Ion Ratio Lower Upper

163 100

194 5.0 3.6 5.4




164 10.9 8.1 12.1

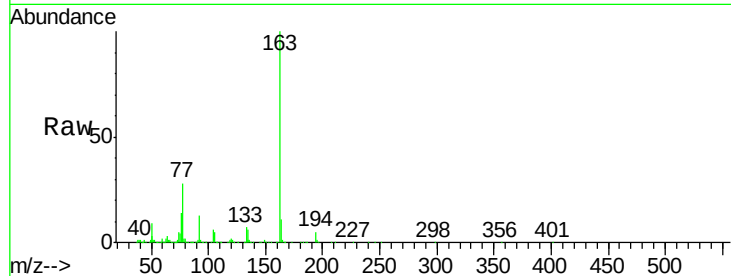

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

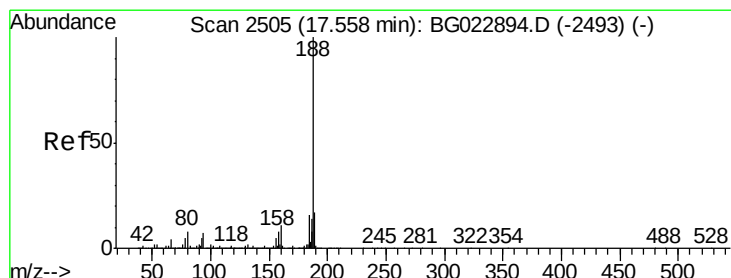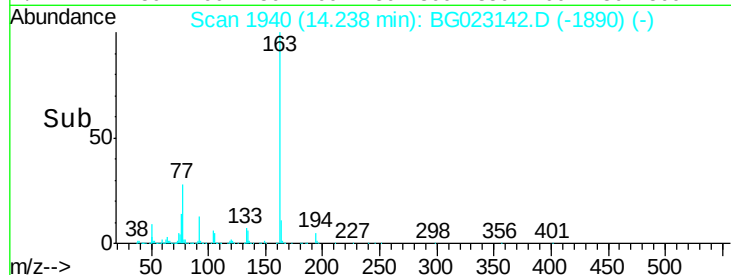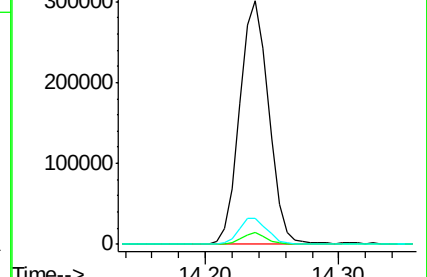

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.55 min Scan# 2504

Delta R.T. -0.01 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38


Tgt Ion:188 Resp: 835321

Ion Ratio Lower Upper

188 100

94 6.7 5.2 7.8



80 10.3 7.2 10.8

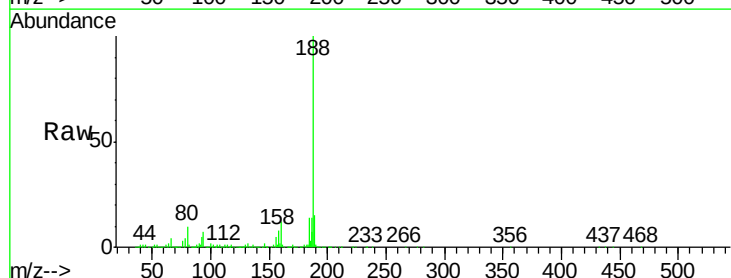


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

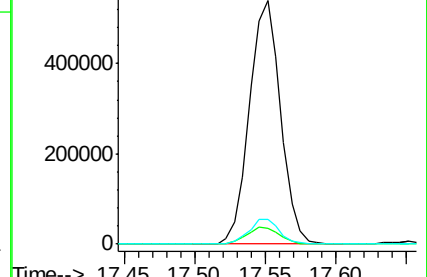

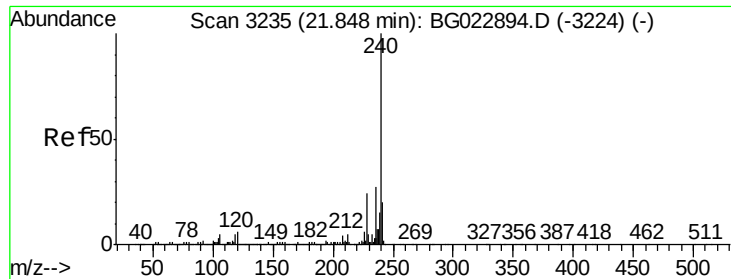

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.85 min Scan# 3236

Delta R.T. 0.00 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38

Instrument :

BNA_G

ClientSampleId :

C5-21


Tgt Ion:240 Resp: 917772

Ion Ratio Lower Upper

240 100

120 6.0 4.1 6.1




236 28.1 21.1 31.7

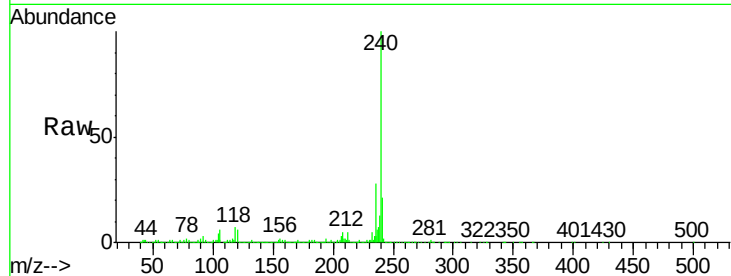

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

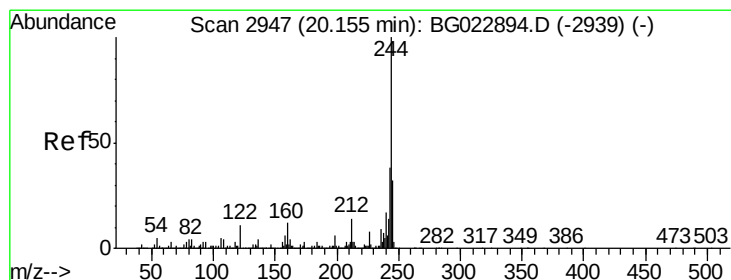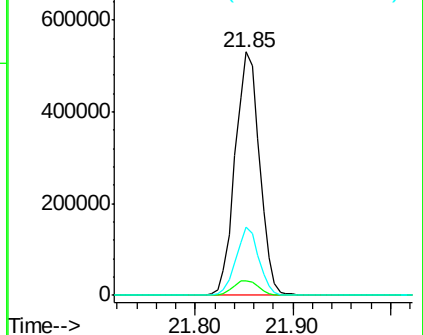

#78

Terphenyl-d14

Concen: 81.94 ng

RT: 20.15 min Scan# 2947

Delta R.T. -0.00 min

Lab File: BG023142.D

Acq: 16 Jul 2016 11:38


Tgt Ion:244 Resp: 2403662

Ion Ratio Lower Upper

244 100

212 12.5 10.8 16.2



122 9.6 8.0 12.0

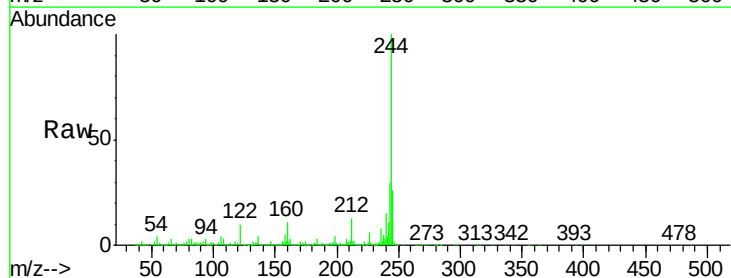


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

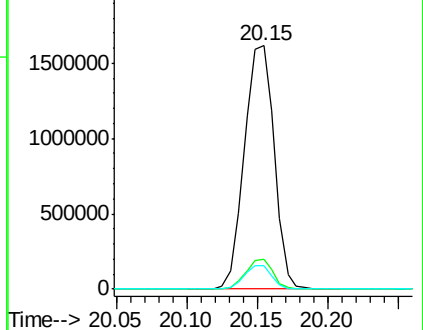

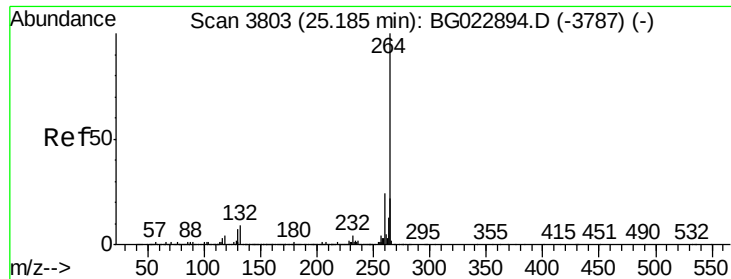

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.22 min Scan# 3810
Delta R.T. 0.04 min
Lab File: BG023142.D
Acq: 16 Jul 2016 11:38

Instrument :
BNA_G
ClientSampleId :
C5-21

Tgt Ion:	264	Resp:	913818
Ion	Ratio	Lower	Upper
264	100		
260	22.2	18.4	27.6
265	22.2	18.9	28.3

