


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071616\
 Data File : BG023138.D
 Acq On : 16 Jul 2016 8:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

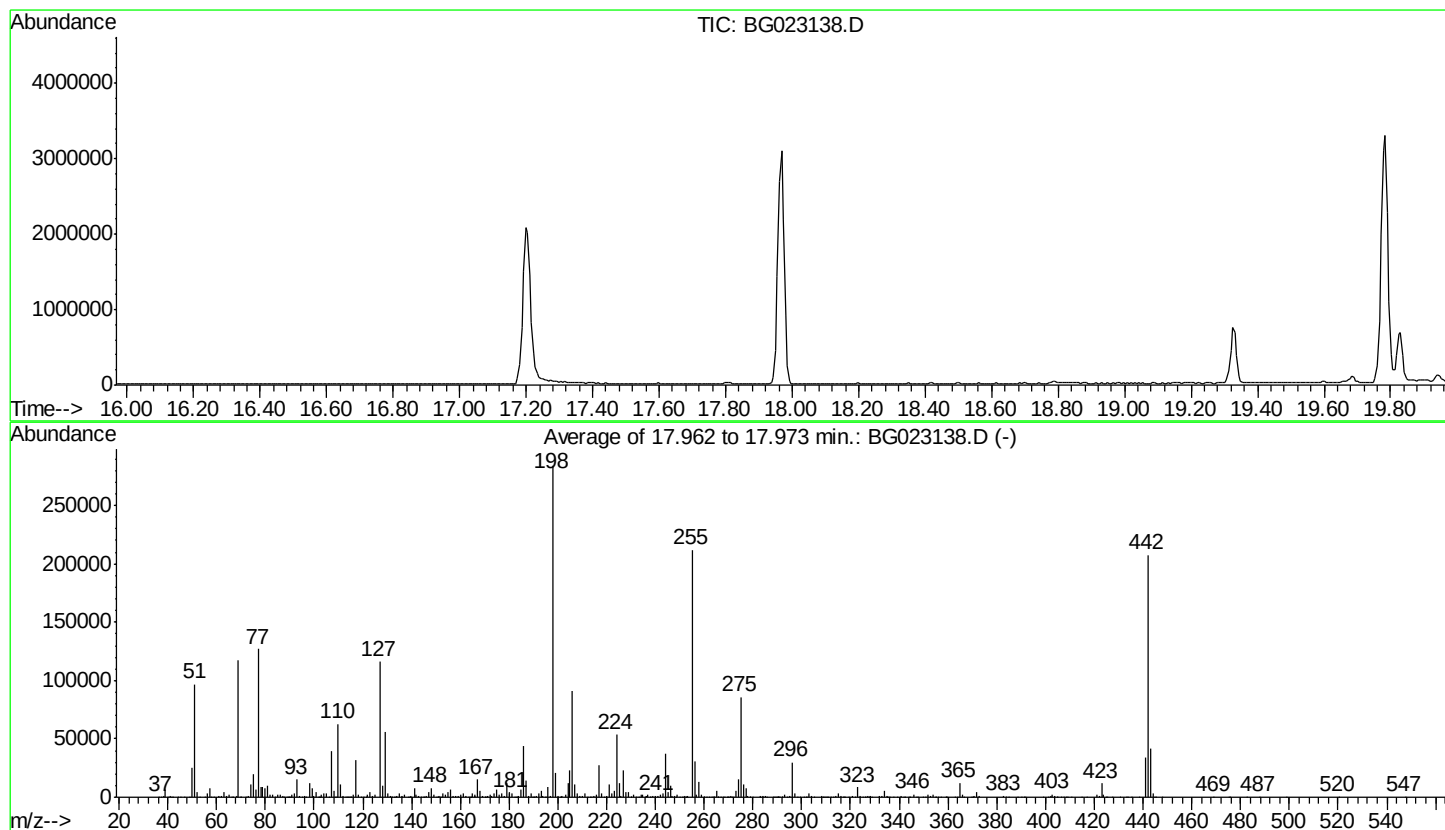

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	96694	PASS
68	69	0.00	2	0.6	743	PASS
69	198	0.00	100	41.4	117792	PASS
70	69	0.00	2	0.5	580	PASS
127	198	10	80	40.9	116157	PASS
197	198	0.00	2	0.5	1459	PASS
198	198	100	100	100.0	284181	PASS
199	198	5	9	7.2	20581	PASS
275	198	10	60	30.2	85752	PASS
365	198	1	100	4.3	12248	PASS
441	442	0.01	24	16.2	33605	PASS
442	198	50	100	73.0	207466	PASS
443	442	15	24	19.9	41226	PASS