

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071624\
 Data File : BG062090.D
 Acq On : 16 Jul 2024 12:10
 Operator : MA/JU
 Sample : PB162022BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	22	26	31	rBV4	12039	19277	1.05%	0.102%
2	3.634	55	59	60	rVB3	2972	3071	0.17%	0.016%
3	3.710	69	72	75	rBV5	3165	3923	0.21%	0.021%
4	3.745	75	78	82	rVB3	2316	3269	0.18%	0.017%
5	3.857	94	97	110	rBV	179792	298833	16.27%	1.583%
6	4.192	151	154	160	rVB4	5096	7264	0.40%	0.038%
7	4.351	178	181	184	rVB2	2428	3364	0.18%	0.018%
8	4.832	262	263	266	rVB2	2653	2500	0.14%	0.013%
9	4.968	282	286	289	rBV	2189	2731	0.15%	0.014%
10	6.131	482	484	487	rBV	2631	2891	0.16%	0.015%
11	6.795	593	597	599	rVB	2413	2946	0.16%	0.016%
12	6.812	599	600	603	rBV	3425	2554	0.14%	0.014%
13	7.218	660	669	676	rBV2	243357	421240	22.94%	2.232%
14	7.265	676	677	679	rVB2	4708	2497	0.14%	0.013%
15	7.371	687	695	703	rBV	160685	252478	13.75%	1.338%
16	7.494	713	716	720	rBV2	1869	2517	0.14%	0.013%
17	7.582	723	731	740	rVV	212114	366695	19.97%	1.943%
18	8.046	803	810	818	rBV	176280	304322	16.57%	1.612%
19	8.205	834	837	841	rBV	2554	3020	0.16%	0.016%
20	8.763	925	932	942	rBV	302898	506399	27.58%	2.683%
21	9.033	975	978	982	rVB2	2088	2475	0.13%	0.013%
22	9.216	1002	1009	1017	rBV	245320	440132	23.97%	2.332%
23	9.362	1031	1034	1037	rVB	3675	4399	0.24%	0.023%
24	9.650	1081	1083	1086	rVB	2585	2696	0.15%	0.014%
25	9.938	1124	1132	1140	rVB	233130	424134	23.10%	2.247%
26	10.179	1169	1173	1178	rVB	2267	3943	0.21%	0.021%
27	10.485	1217	1225	1233	rBV	295702	534558	29.11%	2.832%
28	10.632	1248	1250	1255	rBV	3067	3568	0.19%	0.019%
29	10.861	1283	1289	1300	rVB	280520	498842	27.16%	2.643%
30	10.996	1304	1312	1323	rBV2	315391	595594	32.43%	3.156%
31	11.395	1377	1380	1384	rVB	2342	2540	0.14%	0.013%
32	11.654	1421	1424	1426	rBV	2583	2754	0.15%	0.015%
33	11.789	1445	1447	1450	rBV	2469	2556	0.14%	0.014%
34	12.047	1489	1491	1497	rBV	1885	2810	0.15%	0.015%
35	12.318	1532	1537	1539	rBV	2143	3043	0.17%	0.016%
36	12.435	1552	1557	1559	rBV3	6281	8157	0.44%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071624\
 Data File : BG062090.D
 Acq On : 16 Jul 2024 12:10
 Operator : MA/JU
 Sample : PB162022BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	12.541	1574	1575	1579	rVB	2273	2533	0.14%	0.013%
38	12.753	1608	1611	1614	rBV	1575	2762	0.15%	0.015%
39	13.140	1676	1677	1683	rVB	2896	3301	0.18%	0.017%
40	13.757	1781	1782	1786	rBV	2737	2956	0.16%	0.016%
41	14.080	1829	1837	1844	rBV	720859	1055144	57.46%	5.591%
42	14.310	1874	1876	1879	rBV	3079	3553	0.19%	0.019%
43	14.380	1881	1888	1898	rVB2	625346	986707	53.73%	5.228%
44	14.686	1932	1940	1947	rBV	465973	748813	40.78%	3.968%
45	14.897	1969	1976	1986	rBV	353581	579811	31.57%	3.072%
46	15.379	2056	2058	2061	rVB	3279	2516	0.14%	0.013%
47	15.608	2095	2097	2099	rBV3	3845	2788	0.15%	0.015%
48	15.673	2099	2108	2115	rBV	847906	1256672	68.43%	6.658%
49	15.790	2122	2128	2139	rBV	448525	646111	35.18%	3.423%
50	16.078	2176	2177	2180	rVB3	3251	2761	0.15%	0.015%
51	16.225	2199	2202	2204	rBV3	2134	2599	0.14%	0.014%
52	16.301	2212	2215	2217	rBV2	3786	4084	0.22%	0.022%
53	16.337	2217	2221	2222	rVV2	2849	3135	0.17%	0.017%
54	16.407	2229	2233	2236	rVB2	4225	4461	0.24%	0.024%
55	16.454	2238	2241	2245	rVV2	3341	4135	0.23%	0.022%
56	16.789	2296	2298	2300	rVB3	4465	3042	0.17%	0.016%
57	16.930	2320	2322	2323	rBV	3720	2570	0.14%	0.014%
58	17.324	2385	2389	2390	rBV3	3609	2476	0.13%	0.013%
59	17.429	2400	2407	2413	rBV	726179	1043283	56.81%	5.528%
60	17.529	2416	2424	2431	rBV	1011324	1556158	84.74%	8.245%
61	17.747	2459	2461	2463	rBV2	2557	2478	0.13%	0.013%
62	18.082	2514	2518	2519	rBV3	5495	5646	0.31%	0.030%
63	18.140	2527	2528	2529	rBV	4837	2526	0.14%	0.013%
64	18.657	2614	2616	2618	rBV2	4122	2955	0.16%	0.016%
65	19.368	2734	2737	2743	rVB5	19707	26189	1.43%	0.139%
66	19.445	2746	2750	2755	rVB4	18337	27020	1.47%	0.143%
67	19.539	2765	2766	2768	rBV2	5840	4079	0.22%	0.022%
68	19.809	2806	2812	2825	rBV2	1271831	1836413	100.00%	9.730%
69	21.689	3126	3132	3140	rVB	699054	1159736	63.15%	6.145%
70	24.691	3634	3643	3653	rVB2	684138	1816153	98.90%	9.623%
71	24.909	3672	3680	3693	rVB2	449616	1323896	72.09%	7.015%




Sum of corrected areas: 18873454

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071624\
Data File : BG062090.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

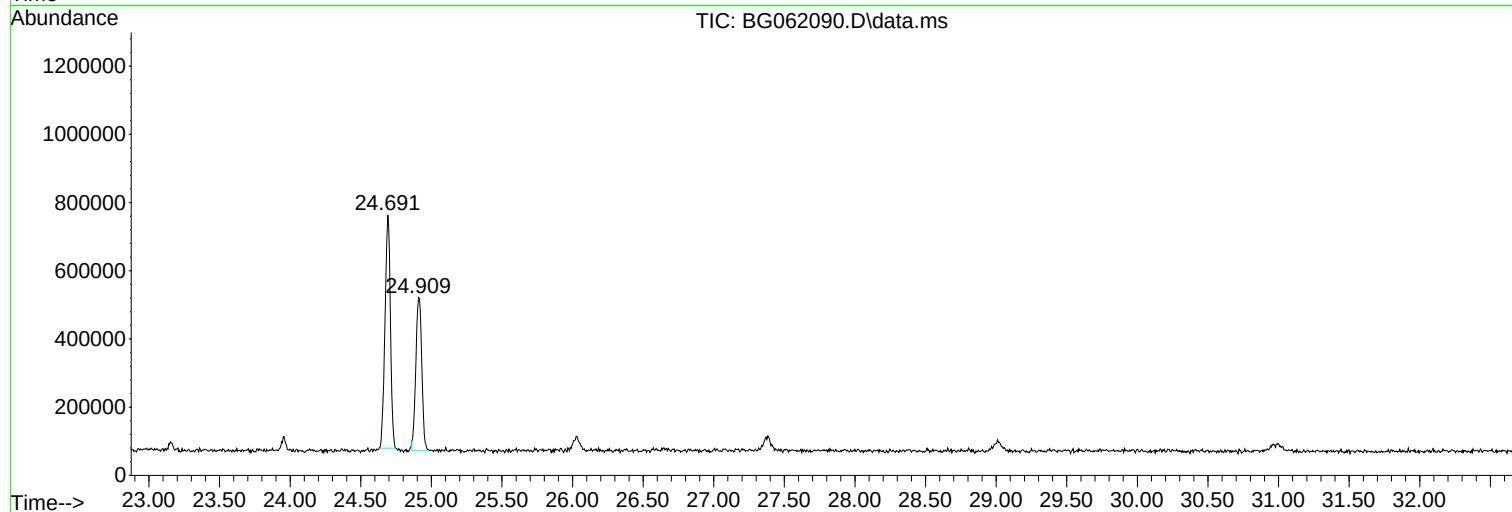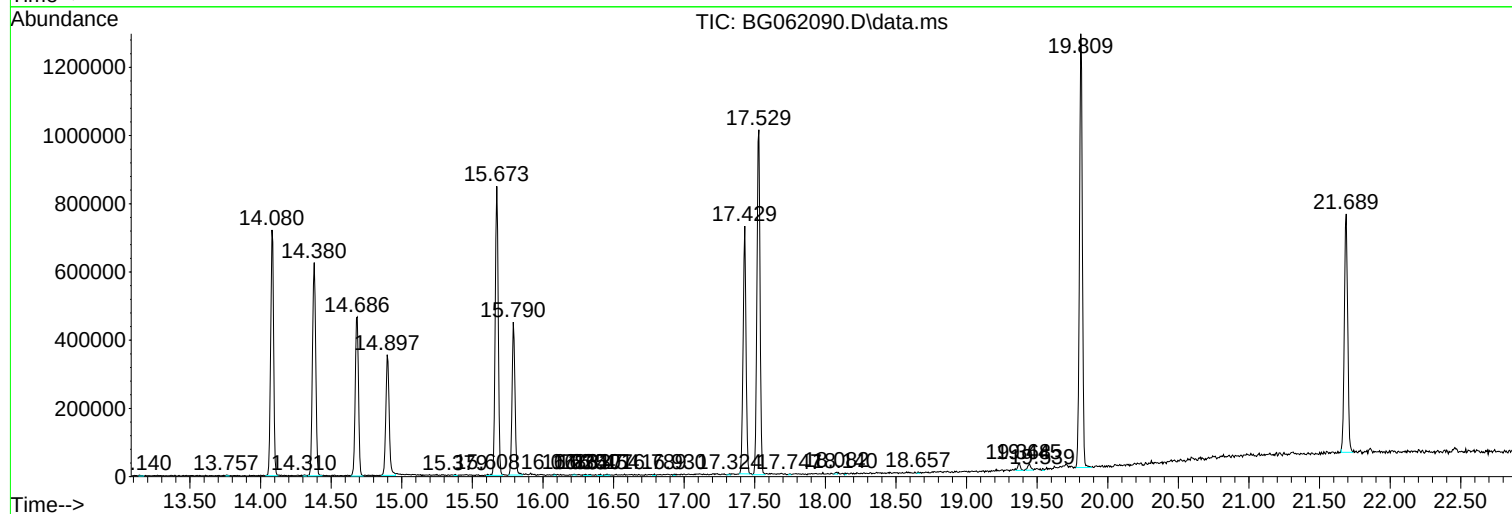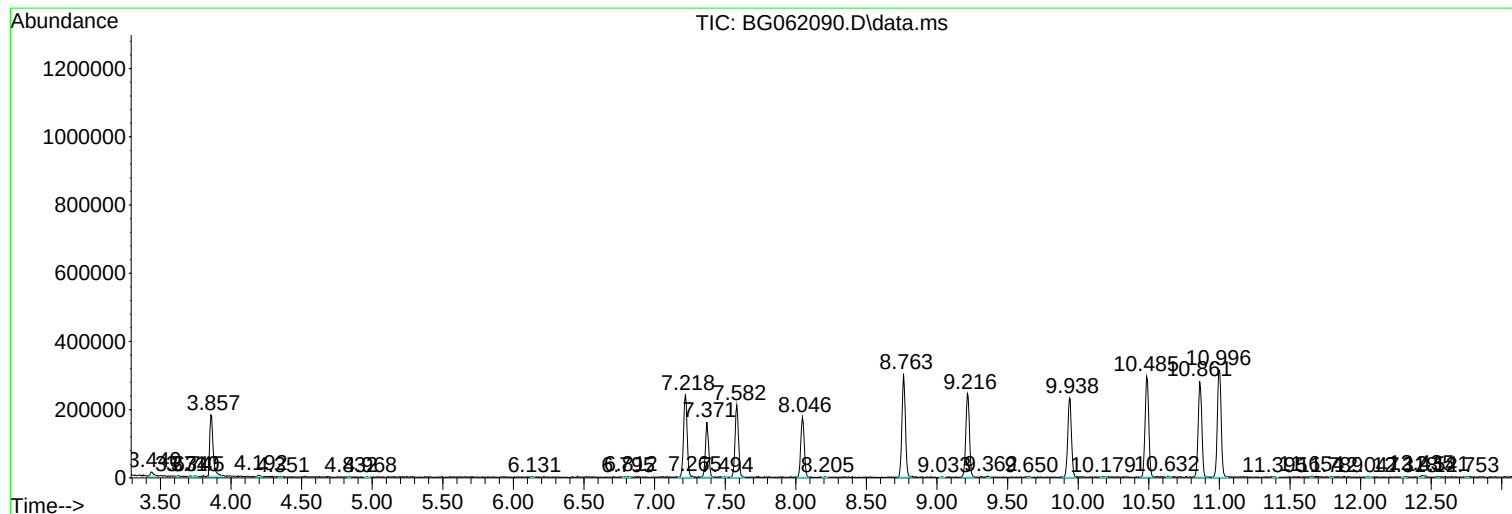

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071624\
Data File : BG062090.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071624\
Data File : BG062090.D
Acq On : 16 Jul 2024 12:10
Operator : MA/JU
Sample : PB162022BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------