
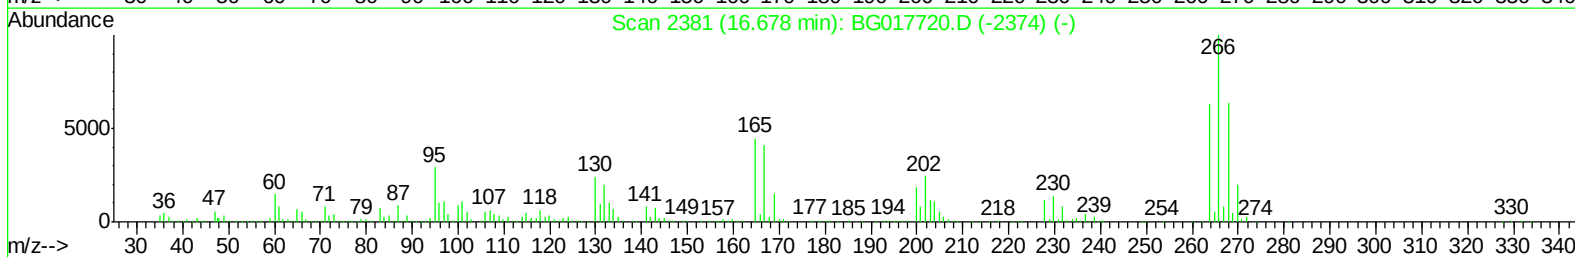
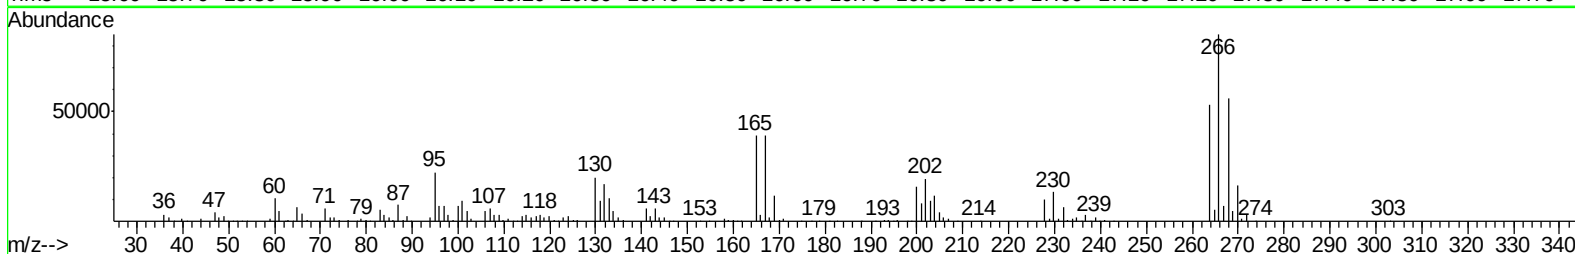


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG071715\  
Data File : BG017918.D  
Acq On : 17 Jul 2015 10:01  
Operator : TP/UM  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:31:13 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG071715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 18 01:50:30 2015  
Response via : Initial Calibration

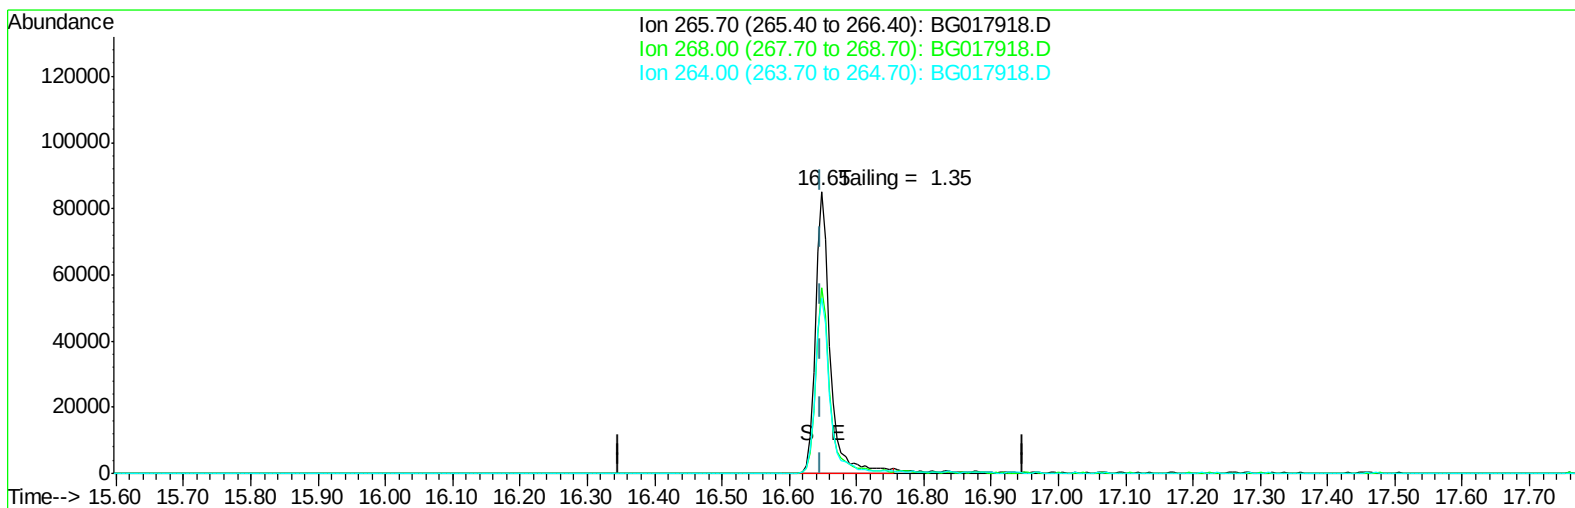

TIC: BG017918.D

(69) Pentachlorophenol (C)




16.648min (+0.001) 5838.50ng

response 131867

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.80 | 66.07 |
| 264.00 | 63.40 | 62.15 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\Data\BG071715\  
Data File : BG017918.D  
Acq On : 17 Jul 2015 10:01  
Operator : TP/UM  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:31:13 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG071715.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 18 01:50:30 2015  
Response via : Initial Calibration

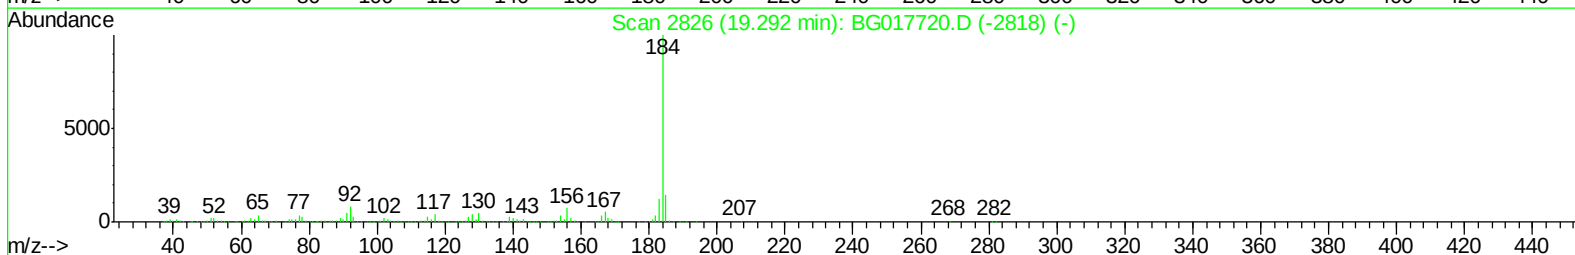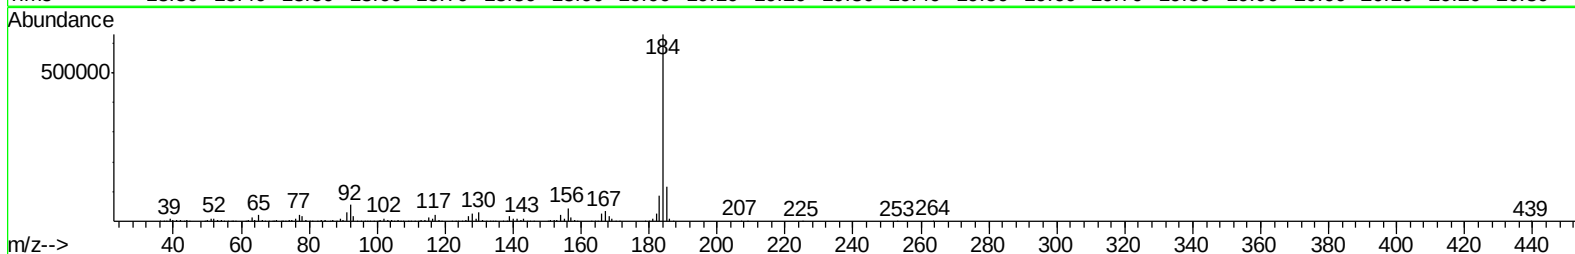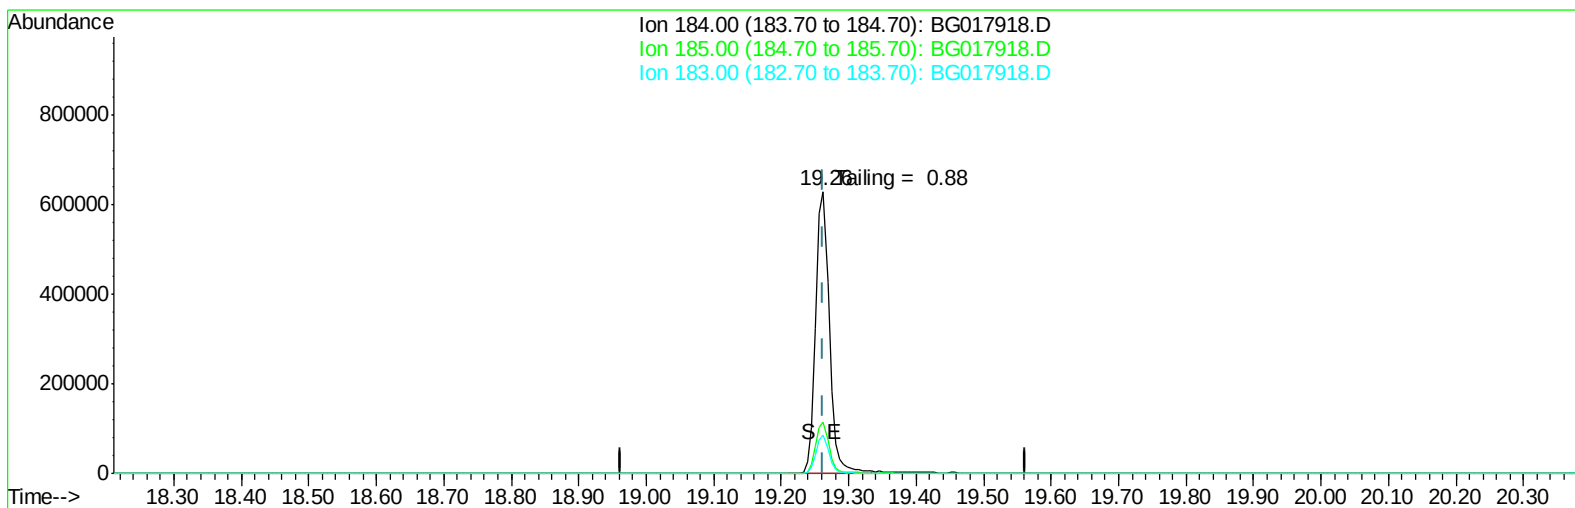

TIC: BG017918.D

(76) Benzidine

19.263min (+0.000) 405126.57ng

response 874436

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 14.40 | 18.23# |
| 183.00 | 12.50 | 13.70  |
| 0.00   | 0.00  | 0.00   |