
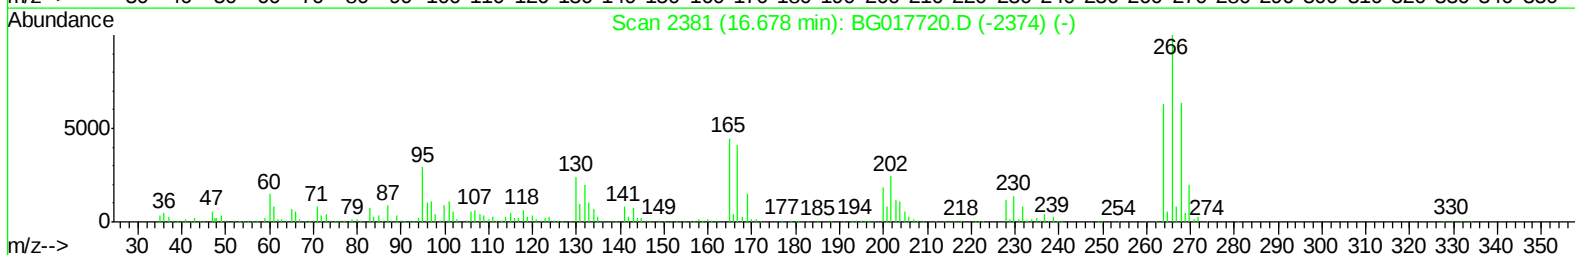
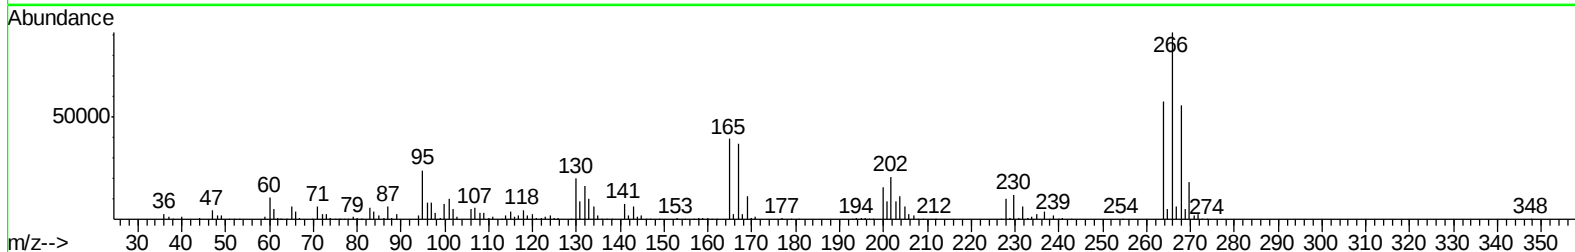


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
Data File : BG017928.D
Acq On : 17 Jul 2015 16:53
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:37:11 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 01:50:30 2015
Response via : Initial Calibration

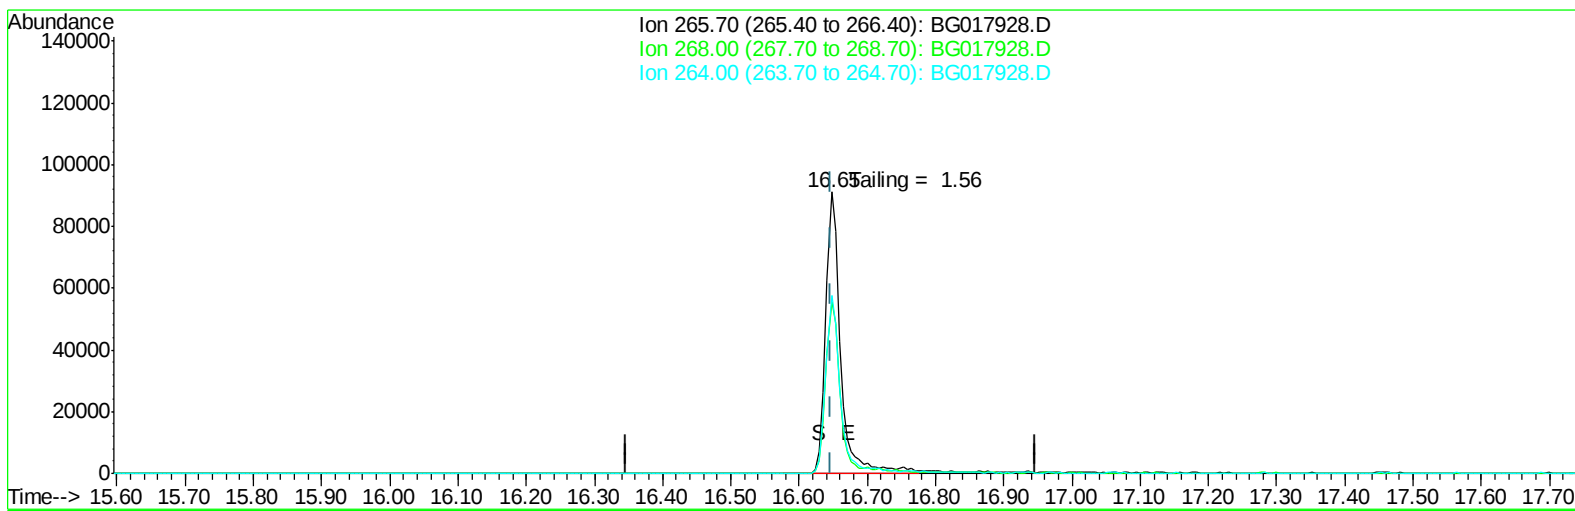

TIC: BG017928.D

(69) Pentachlorophenol (C)




16.647min (+0.000) 3580.75ng

response 133469

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	61.14
264.00	63.40	63.28
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
Data File : BG017928.D
Acq On : 17 Jul 2015 16:53
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:37:11 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 01:50:30 2015
Response via : Initial Calibration

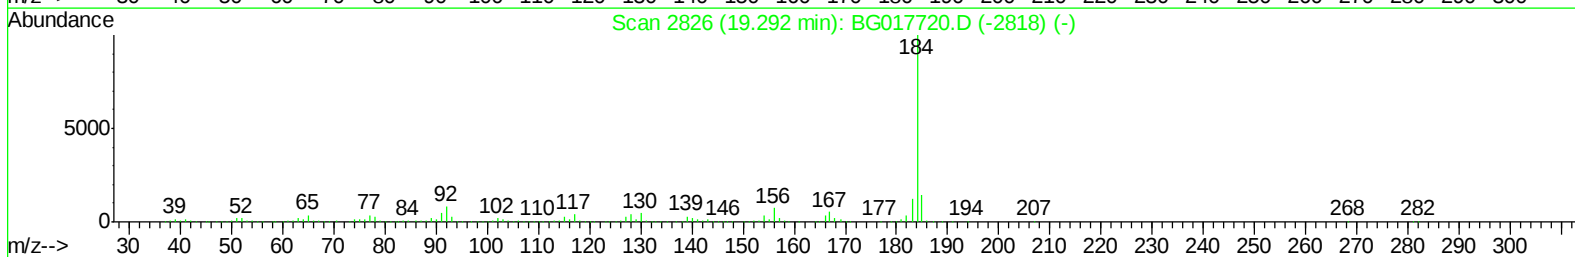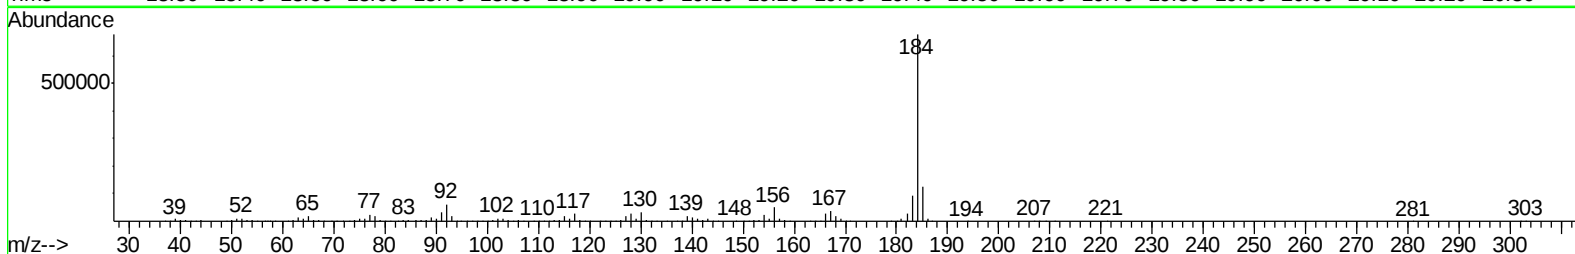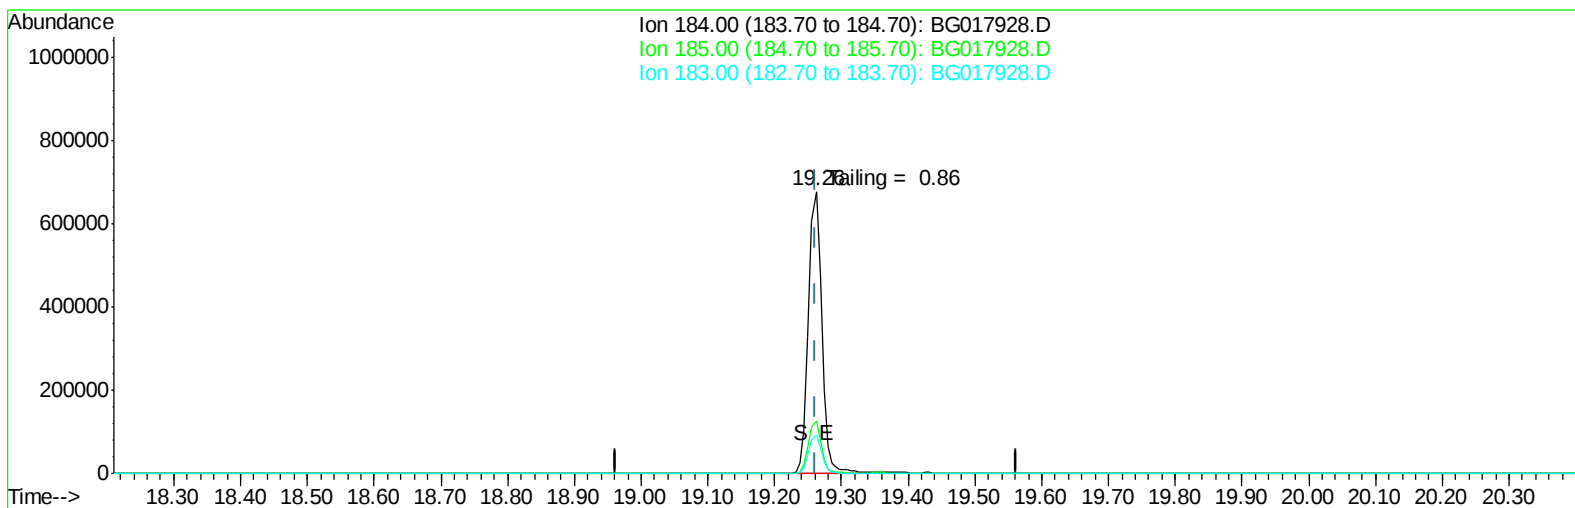

TIC: BG017928.D

(76) Benzidine

19.262min (-0.001) 60237.42ng

response 920391

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	18.46#
183.00	12.50	13.70
0.00	0.00	0.00