
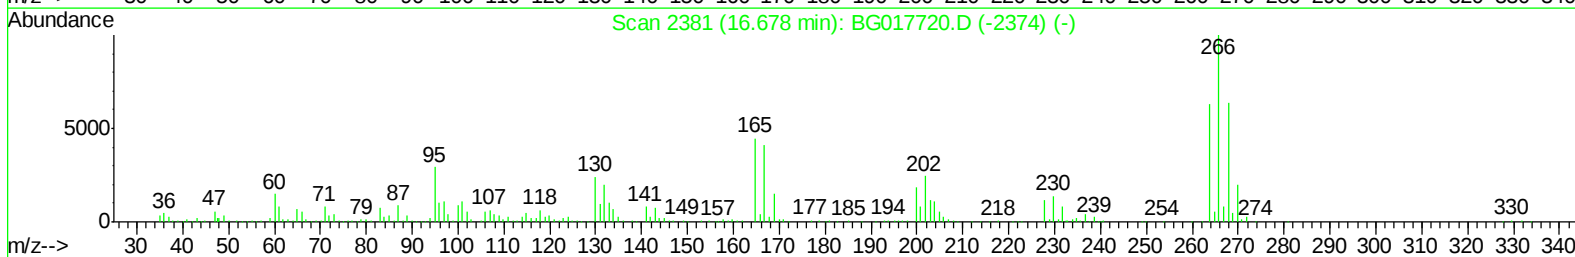
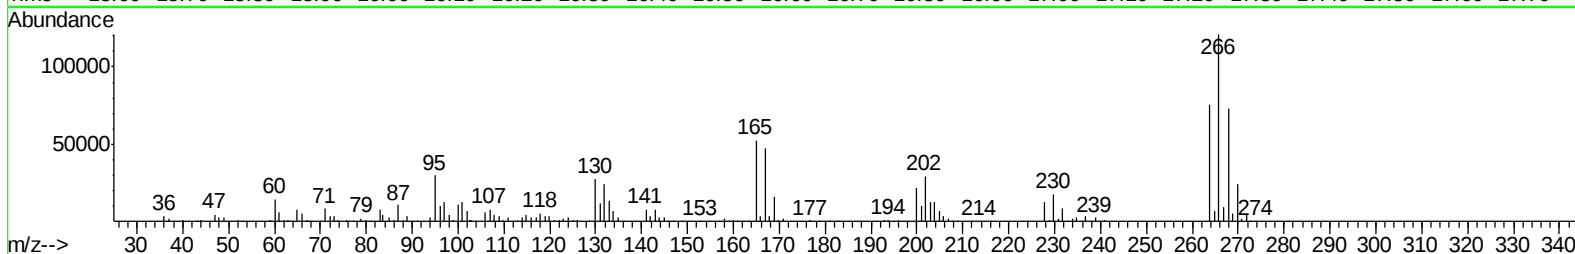


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
Data File : BG017946.D
Acq On : 18 Jul 2015 4:10
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:42:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 01:50:30 2015
Response via : Initial Calibration

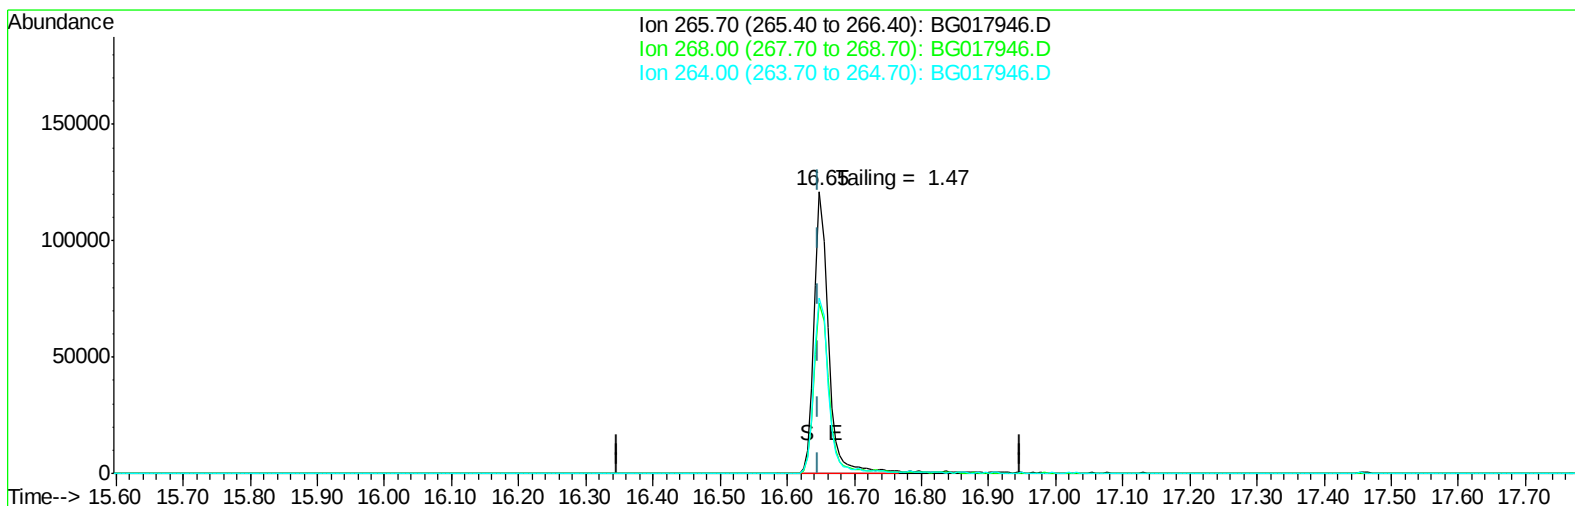

TIC: BG017946.D

(69) Pentachlorophenol (C)




16.648min (+0.001) 7544.17ng

response 175106

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	60.63
264.00	63.40	62.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
Data File : BG017946.D
Acq On : 18 Jul 2015 4:10
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 09:42:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 01:50:30 2015
Response via : Initial Calibration

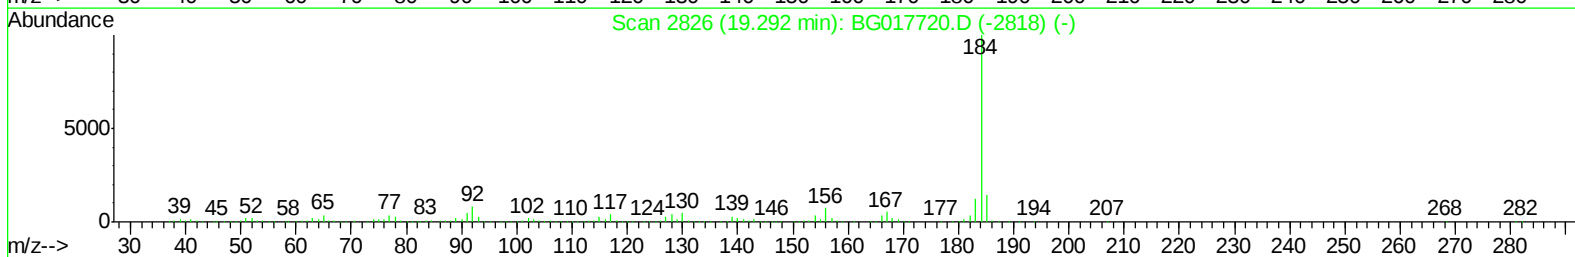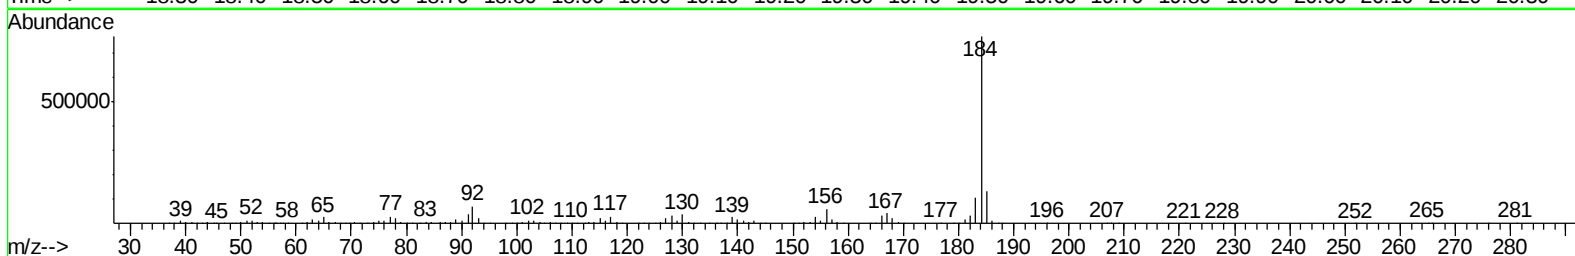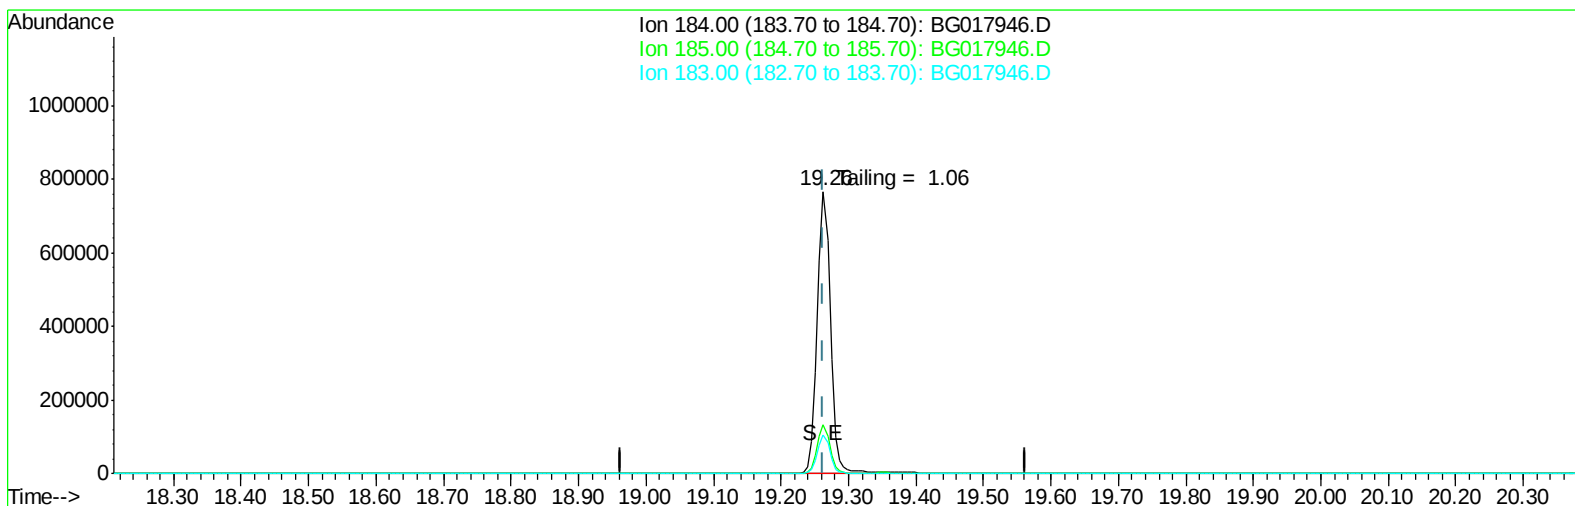

TIC: BG017946.D

(76) Benzidine

19.263min (+0.000) 597547.78ng

response 1018234

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	17.18
183.00	12.50	13.81
0.00	0.00	0.00