


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
 Data File : BG071918.D
 Acq On : 17 Jul 2015 10:01
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

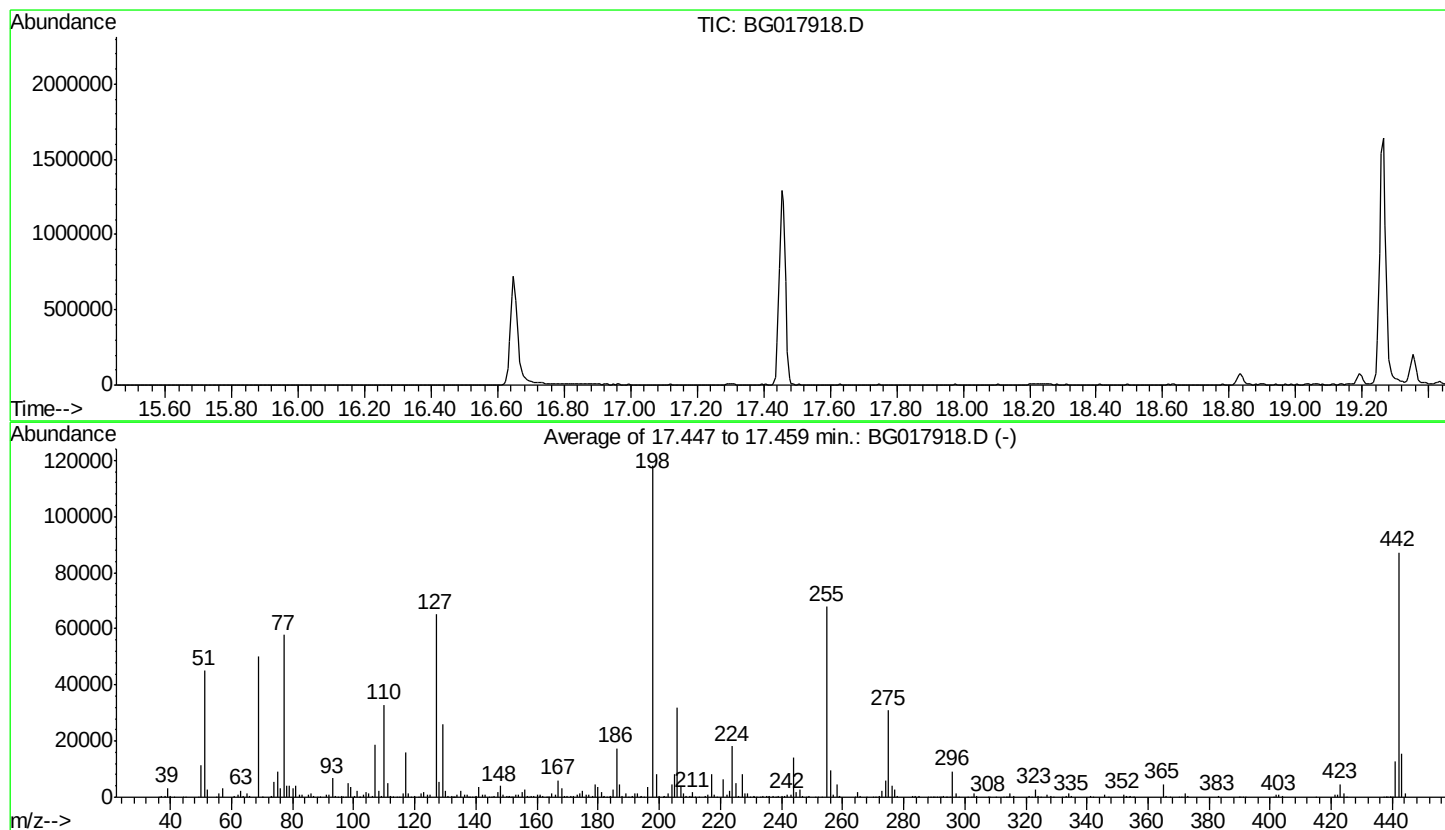

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	45090	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.5	50189	PASS
70	69	0.00	2	0.4	197	PASS
127	198	10	80	55.2	65205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118125	PASS
199	198	5	9	6.9	8176	PASS
275	198	10	60	26.2	30938	PASS
365	198	1	100	3.9	4659	PASS
441	442	0.01	24	14.8	12874	PASS
442	198	50	100	73.8	87192	PASS
443	442	15	24	17.7	15450	PASS