


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
 Data File : BG017928.D
 Acq On : 17 Jul 2015 16:53
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

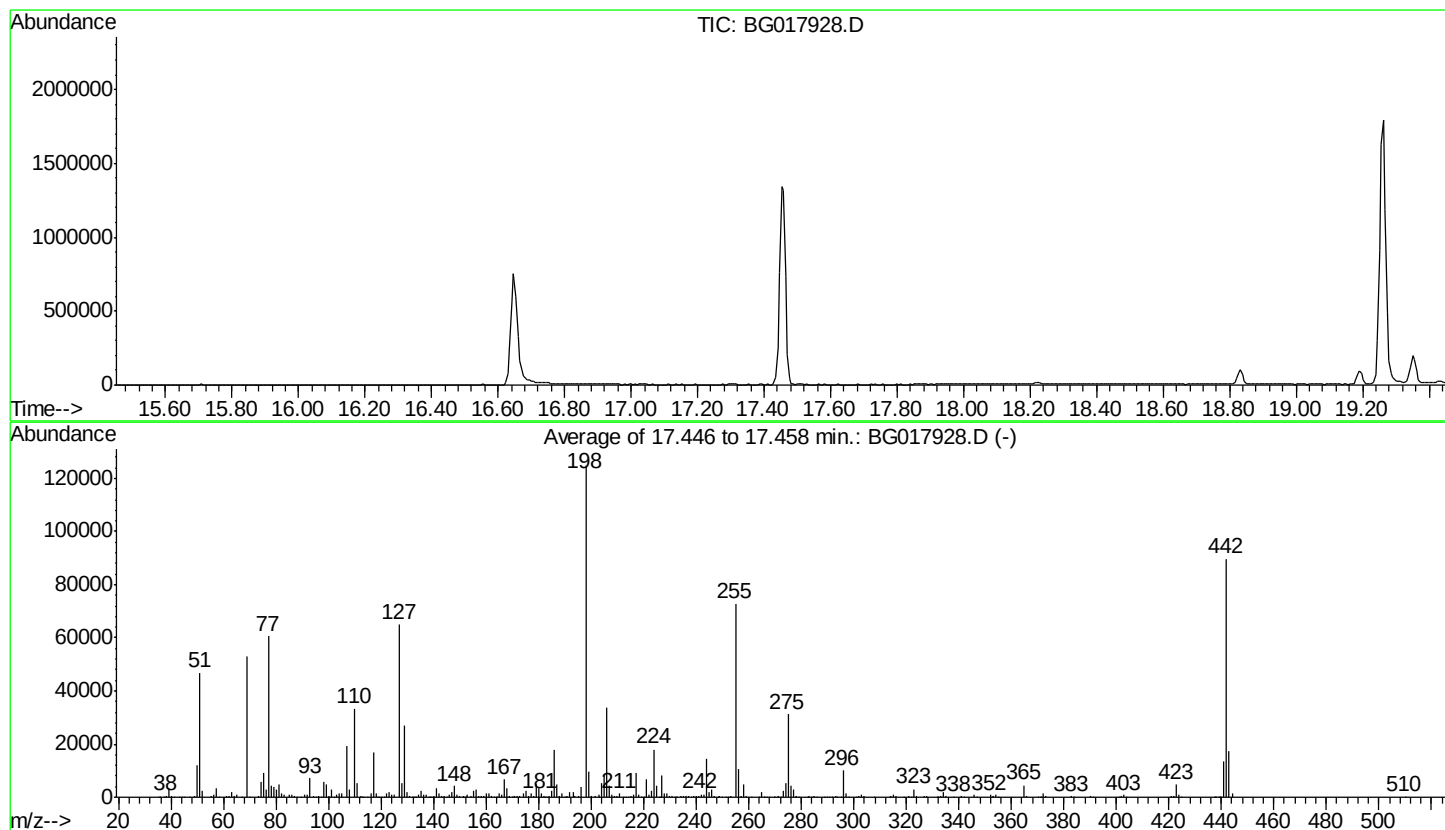

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	46816	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.4	52954	PASS
70	69	0.00	2	0.5	246	PASS
127	198	10	80	52.1	64992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124808	PASS
199	198	5	9	7.6	9469	PASS
275	198	10	60	25.0	31141	PASS
365	198	1	100	3.6	4496	PASS
441	442	0.01	24	14.9	13354	PASS
442	198	50	100	72.0	89864	PASS
443	442	15	24	19.5	17518	PASS