


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071715\
Data File : BG017946.D
Acq On : 18 Jul 2015 4:10
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 19 06:05:07 2015

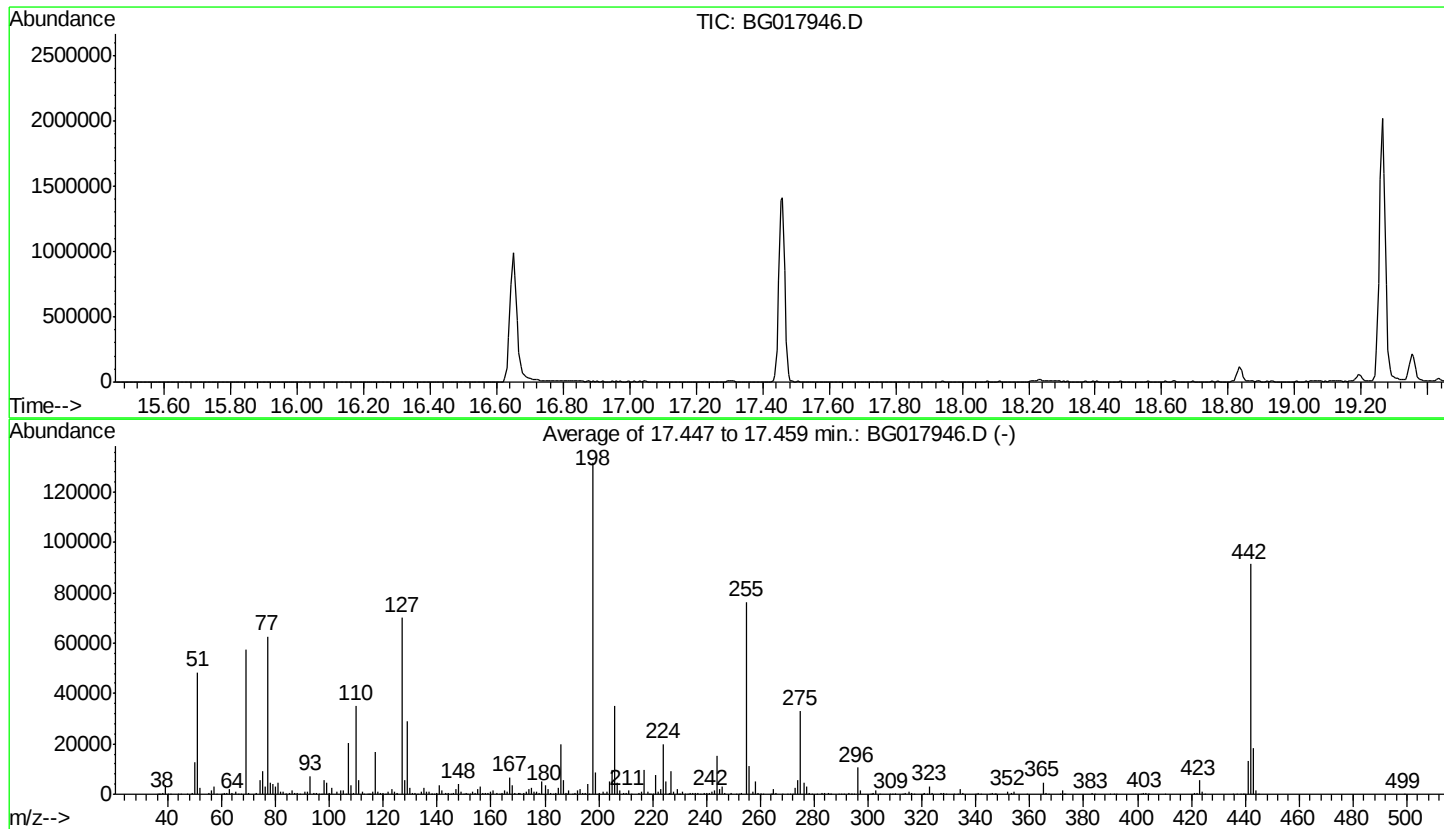

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	48341	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.6	57432	PASS
70	69	0.00	2	0.5	312	PASS
127	198	10	80	53.2	70032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	131706	PASS
199	198	5	9	6.7	8829	PASS
275	198	10	60	25.1	33098	PASS
365	198	1	100	3.6	4708	PASS
441	442	0.01	24	14.6	13360	PASS
442	198	50	100	69.3	91338	PASS
443	442	15	24	19.9	18154	PASS