

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071717\
 Data File : BG027951.D
 Acq On : 17 Jul 2017 16:22
 Operator : SJ/JU
 Sample : PB100660BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK60

Quant Time: Jul 17 16:59:57 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 17 16:40:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	55430	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	231755	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	162617	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.73	188	422932	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	508289	20.00	ng/ul	0.00
83) Perylene-d12	25.58	264	478332	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.87	96	6202	6.17	ng/uL	0.00
5) Phenol-d5	7.51	99	138639	30.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	83883	31.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	114448	31.98	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	111689	29.62	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	55347	32.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	65723	32.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.81	165	122653	30.55	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	156816	43.21	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	486212	34.49	ng/ul	0.00
46) Acenaphthylene-d8	14.68	160	514151	32.08	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	50672	24.82	ng/ul	0.00
57) Fluorene-d10	15.97	176	426062	32.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.08	200	77707	26.45	ng/ul	0.00
70) Anthracene-d10	17.83	188	699601	34.30	ng/ul	0.00
76) Pyrene-d10	20.10	212	812884	35.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.34	264	758004	33.93	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	9.05	70	2761	1.013	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071717\
Data File : BG027951.D
Acq On : 17 Jul 2017 16:22
Operator : SJ/JU
Sample : PB100660BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK60

Quant Time: Jul 17 16:59:57 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 17 16:40:57 2017
Response via : Initial Calibration

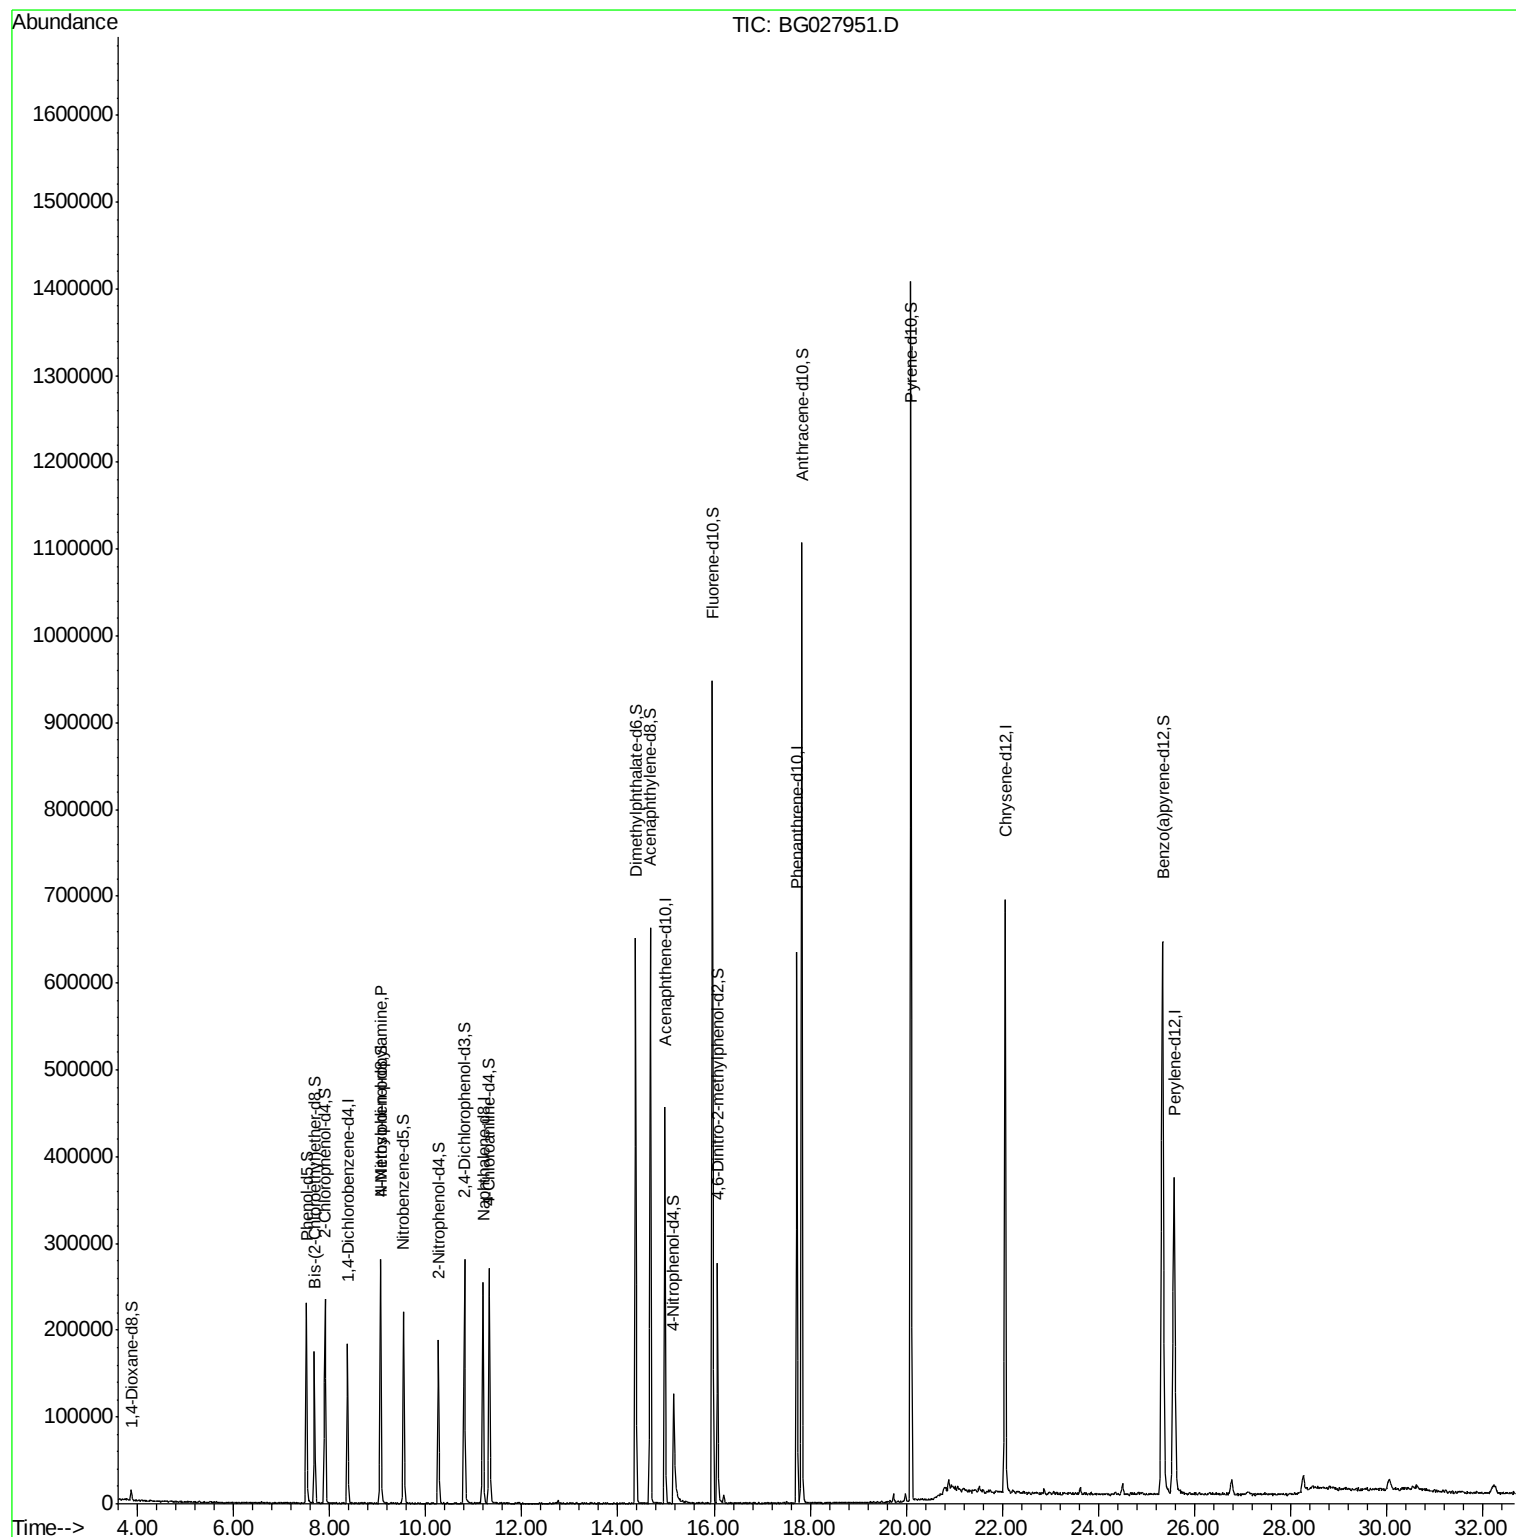

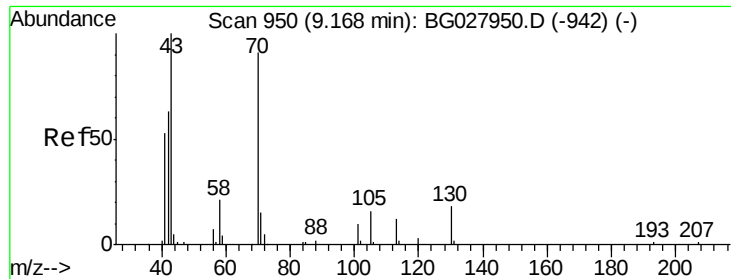

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.013 ng/ul
 RT: 9.05 min Scan# 930
 Delta R.T. -0.11 min
 Lab File: BG027951.D
 Acq: 17 Jul 2017 16:22

Instrument :
 BNA_G
 ClientSampleId :
 SBLK60

Tgt Ion: 70 Resp: 2761
 Ion Ratio Lower Upper
 70 100
 42 469.3 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

