

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071717\
 Data File : BG027952.D
 Acq On : 17 Jul 2017 17:02
 Operator : SJ/JU
 Sample : PB100641BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK41

Quant Time: Jul 17 17:41:03 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 17 16:40:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	52422	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	211893	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.97	164	148276	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	390679	20.00	ng/ul	0.00
75) Chrysene-d12	22.05	240	475123	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	450952	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.86	96	7572	7.96	ng/uL	0.00
5) Phenol-d5	7.52	99	148990	34.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	91544	36.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.91	132	126446	37.36	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	128782	36.11	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	59520	38.18	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	74599	39.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	135285	36.86	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	170896	51.51	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	519239	40.39	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	563226	38.55	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	56596	30.40	ng/ul	0.00
57) Fluorene-d10	15.96	176	462962	38.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	87798	32.36	ng/ul	0.00
70) Anthracene-d10	17.82	188	758629	40.27	ng/ul	0.00
76) Pyrene-d10	20.09	212	892007	41.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	851204	40.41	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	9.06	70	3382	1.312	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071717\
Data File : BG027952.D
Acq On : 17 Jul 2017 17:02
Operator : SJ/JU
Sample : PB100641BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK41

Quant Time: Jul 17 17:41:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 17 16:40:57 2017
Response via : Initial Calibration

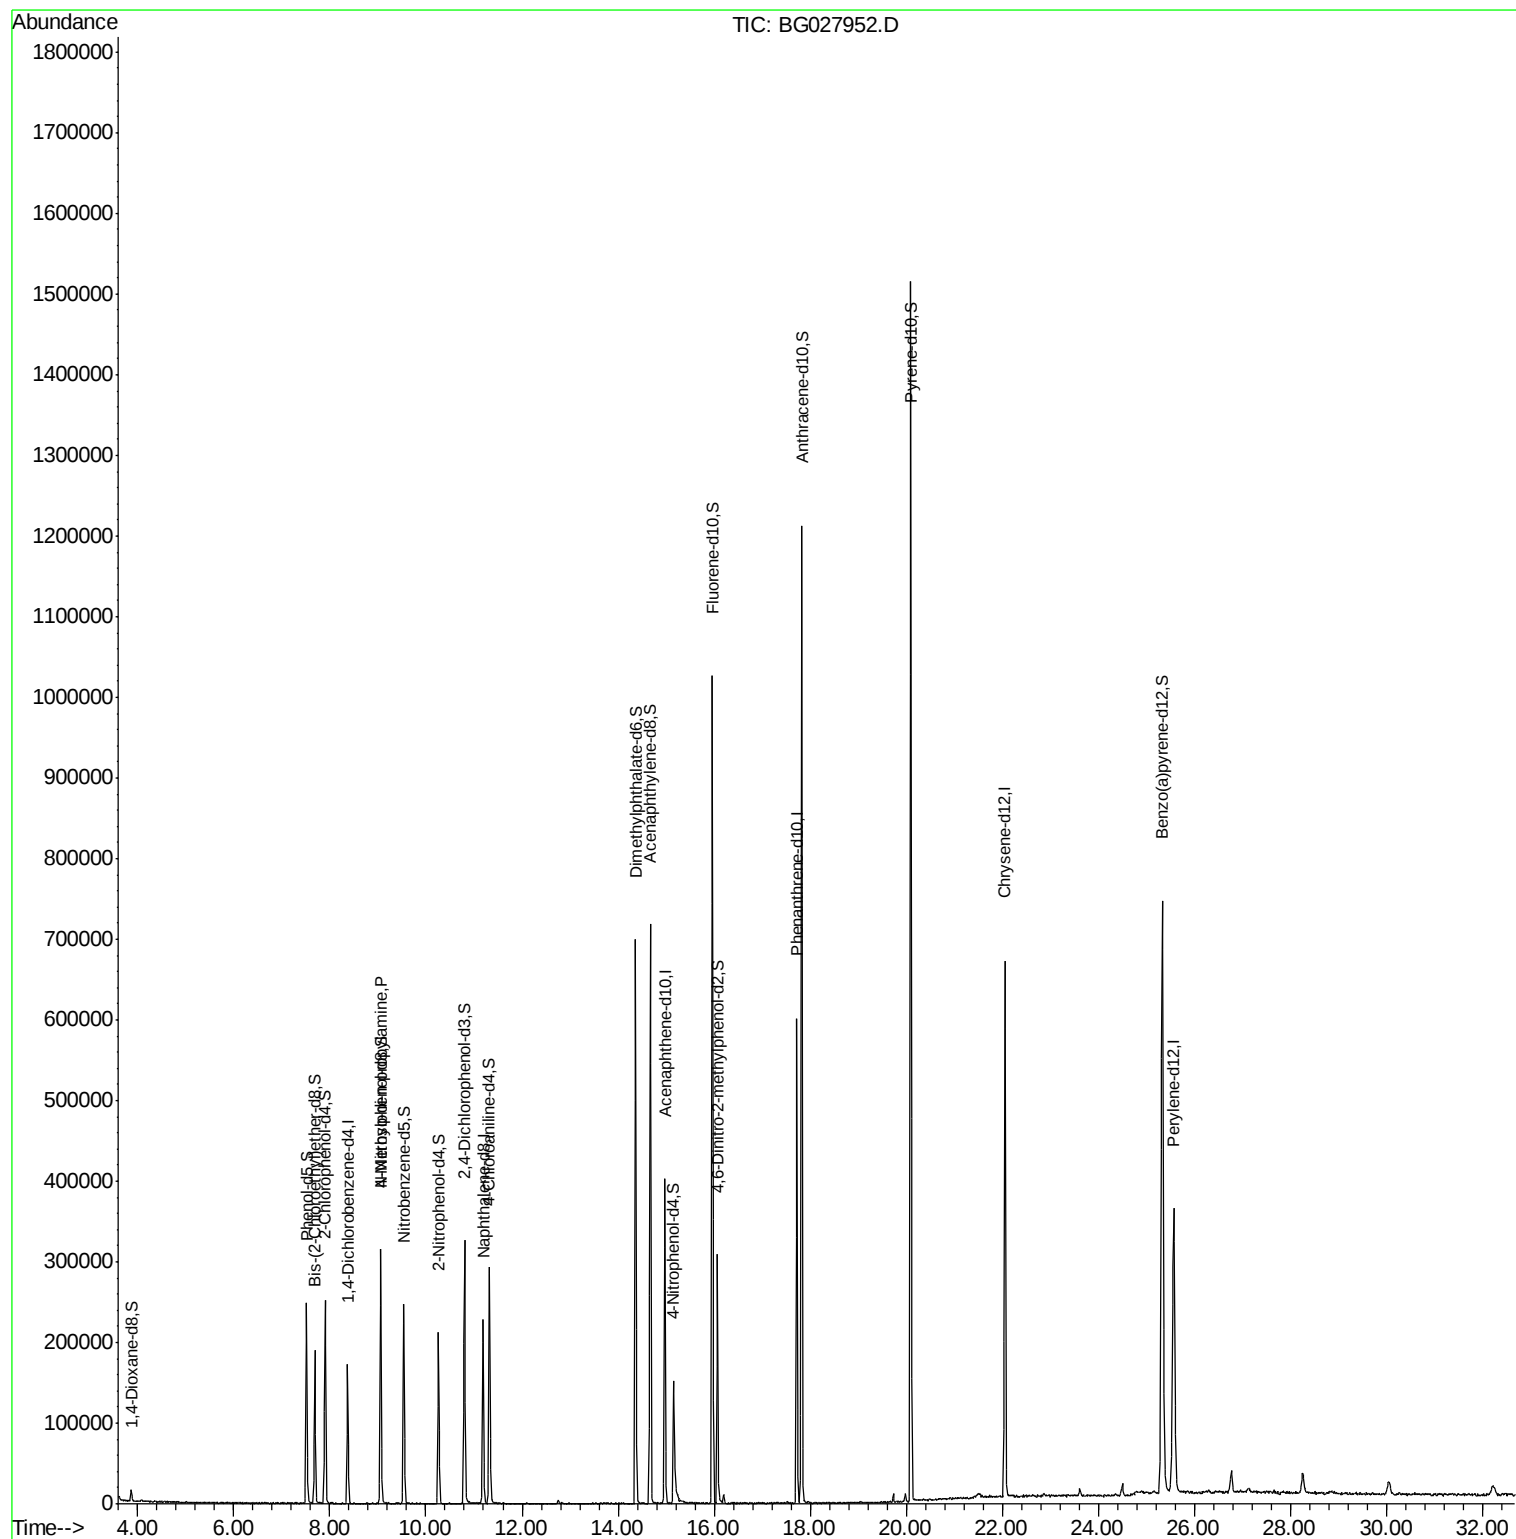

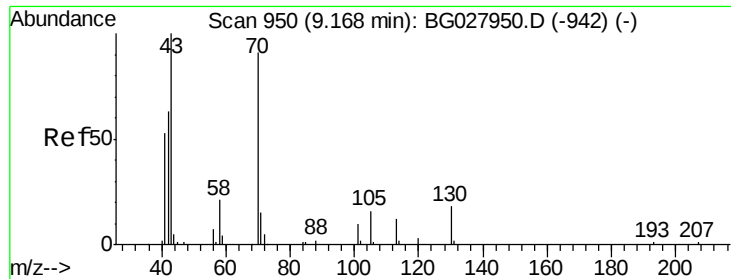

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.312 ng/ul
 RT: 9.06 min Scan# 931
 Delta R.T. -0.11 min
 Lab File: BG027952.D
 Acq: 17 Jul 2017 17:02

Instrument :
 BNA_G
 ClientSampleId :
 SBLK41

Tgt Ion: 70 Resp: 3382
 Ion Ratio Lower Upper
 70 100
 42 363.5 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

